



Manual

PICO-PROFILE with PICO-T3PN Segments



Thank you for purchasing a IMKO instrument.

Should you have any queries please
don't hesitate to contact your local
distributor or address directly to IMKO:

IMKO Micromodultechnik GmbH

Im Stoeck 2
D-76275 Ettlingen
Germany

Phone: +49-7243-5921-0

Fax: +49-7243-90856

E-mail: info@imko.de

Internet: <http://www.imko.de>

Manual for TRIME[®]-PICO PROFILE

status 16 February 2015

List of contents

1	Functional Description	6
1.1	Operation modes	6
1.1.1	Operation mode A (Bus communication)	6
1.2	External power supply	7
1.3	Installation hints.....	7
2	Technical Data.....	8
2.1	Probe length, spacers and TECANAT access tube.....	9
2.2	How to connect PICO-T3PN with connection tube set	10
2.3	PICO DataLogger cable 5m or 15m length	11
2.4	PICO DataLogger cable 25m, 50m or 100m length	11
2.5	PICO IMP-Bus cable 5m, 4-pin female connector (Item no.: 300115).....	11
2.6	Accessories - SM-USB (Converter Module), (Item no.: 100020).....	12
3	Access Tubes and Augers.....	13
3.1	Instructions for Access Tube Installation	14
3.2	Inserting and Fixing the Rubber Bung.....	14
3.3	Instructions for Water Proof Installation	16
4	Remote Power Supply to TRIME PICO-PROFILE	17
5	Datalogging configuration examples	18
5.1	PICO probes connected to the GlobeLog data logger via the IMP-Bus	18
5.2	PICO probes connected to a PC under Windows	19
5.3	PICO probes connected to SDI12 dataloggers	20
6	Information on Lightning Protection of a Sensor Network (IMP-Bus, GlobeLog Logger and integrated Sensors).....	21
6.1	Introduction	21
6.2	Excess voltage protection on 110/220V mains supply.....	21
6.3	Protection of modem and telephone lines	21

6.4	Excess voltage protection for network modules by "SM-Blitz"	21
6.5	Lightning protection on meteorological towers.....	21
6.6	Installation instructions for SM BLITZ lightning protection modules	21
6.7	Conclusion	22
7	TRIME PICO-T3PN theory	23
7.1	Introduction.....	23
7.2	Measuring Field.....	23
7.3	Measuring experiences	24
7.4	Summary.....	24
8	Basic Calibration with the Calibration Set	25
8.1	What is a basic calibration?	25
8.2	What are the benefits of the calibration set for the user?	25
8.2.1	Calibration set for TRIME probes	25
8.3	How to perform a basic calibration?	26
8.3.1	Preparation of the glass beads.....	26
8.3.2	Basic calibration procedure	26
8.3.3	Material specific calibration.....	27
9	TRIME WIN MONITOR.....	28
9.1	Installation	28
9.2	Connect Trime-PICO to a PC	28
9.3	Operating the program	28
9.4	Explanation of measuring data.....	34
9.5	File format.....	35
10	Quick guide for the Software PICO-CONFIG.....	36
10.1	Connection of the RS485 or the IMP-Bus to the SM-USB Module.....	36
10.2	Bus Configuration and Probe Scan	38
10.3	Scan of connected PICO probes on the serial interface	38
10.4	Configuration of Measure Mode	39
10.5	Analogue outputs of the PICO probe	39
10.6	Simulate Analog Output	40
10.7	Selection of the individual Calibration Curves	40
10.8	Test Run in Measurement Mode A	41
10.9	Calibration Curves	43
10.10	Creating a linear Calibration Curve for a specific Material	47
10.11	Nonlinear calibration curves	47
11	Electrical Conductivity with TRIME Probes.....	49

11.1	The analysis of Soils for Electrical Conductivity EC _{TRIME}	50
11.2	EC _{TRIME} Measurement Range for TRIME Probes	50
11.3	Measurement of Pore-Water-Conductivity or Salt-Content of Soils.....	51
11.4	Creation of a Moisture/ EC _{TRIME} Diagram for a particular Soil	54
12	Software Error codes	55
12.1	Software Errors which will be coded with 4 digits.....	55
12.2	PICO Errors (Firmware errors).....	57

1 Functional Description

The intelligent and compact TRIME PICO-PROFILE sensors are measurement devices for continuous and non-destructive determination of volumetric moisture. They are designed for stationary subterranean field use. A variety of installation options (greater depth, vertical or horizontal orientation) offer a wide range of applications.

TRIME PICO-PROFILE systems require an external 7-24V/DC power supply. They are designed for connection to a data logger or a PC for monitoring and data logging purposes.

Your sensor is supplied ready for use and works in a wide range of standard soils. For further information please check the details under Section 6!

1.1 Operation modes

TRIME PICO-PROFILE systems are supplied with a RS485 or IMP-Bus interface and have no analogue outputs.

TRIME PICO-PROFILE sensors can be easily connected to an IMKO GlobeLogger (Operation mode A). A detailed description of how to select a specific operation mode for your application can be found below.

1.1.1 Operation mode A (Bus communication)

TRIME PICO-PROFILE systems can be connected directly to the RS485 bus or IMP-Bus (4-wire bus system), either via IMKO's GlobeLog datalogger or via the SM-USB level converter module for use in conjunction with the TRIME WIN MONITOR data-logging software.

If multiple sensors are to be wired as a network, IMKO offers 3-port, 6-port and 12-port distribution modules. Please note that the IMP-Bus cable length and cable diameter must be properly matched as otherwise the energy consumption of the TRIME sensors (100mA @ 12V/DC for 2..3s) may cause a drop in voltage. *More information is available in Section 5.*

► Benefits:

- Extremely low power consumption in field installations (with GlobeLogger)
- Straightforward installation and simple wiring by virtue of pre-configured standard components (e.g. lightning protection, distribution modules...)
- Systems are supplied ready for use
- Cable length >1000m (with only 4 wires for all sensors)

► For use with:

- GlobeLogger
- PC under Windows with the software TRIME WIN MONITOR, only with converter module SM-USB.
- IMKO calibration and test software PICO-CONFIG (see page 27, Software download: www.imko.de) only with converter module SM-USB.

1.2 External power supply

In the IMP-Bus the power to sensors can be supplied by battery, a complete solar system or mains power. For serial connection of a large number of sensors (up to 150 sensors) or very long IMP232-bus cables up to 1km it is advisable to use a power amplifier module (SM-23LV) or decentralised power supply.


1.3 Installation hints

Please assure careful installation of the probes with close contact between rod and soil. It is important to avoid air pockets around the rods as the highest measuring sensitivity is directly around them.

Air pockets around the probe rods can reduce the measured moisture reading. Where saturated soils are involved, water-filled air pockets will result in an exaggerated reading.


IMKO supplies pre-drilling sets for an optimal preparation of the installation point avoiding compaction of soil otherwise caused by the insertion of the rods.

2 Technical Data

Technical Data	
	
Measuring Segment PICO-T3PN	
Power supply:	7V..24V-DC
Power consumption:	100mA @ 12V/DC during 2..3sec. of measuring
Moisture measuring range:	0..100% volumetric water content
Accuracy (in % volumetric water content):	± 2%
Repeating accuracy/reproducibility:	< 0,1%
Conductivity measuring range:	EC _w 0...>20dS/m
Measurement volume:	1dm ³
Operating Temperature:	-15°C...50°C (extended temperature range on request)
Calibration:	Selectable calibration curves: 1. Standard calibration (soil ±3%) 2. Sand 3. Clay 4. Loam 5. Dielectric Permittivity
Probe body:	waterproof sealed PVC (IP62)
Size:	210 x Ø 40mm
Access tube:	Tecanat ø44mm, max. 3m length
Connection tube set between two PICO-T3PN segments:	Made of aluminium and PVC. Incl. BCS6 male-connector and female-connector. Available lengths: 10cm, 30cm and 80cm, special lengths on request!
Interfaces:	IMP-BUS or SDI12 R485 on request
Cable:	2m, 5m and 10m cable with 4-pin female connector


2.1 Probe length, spacers and TECANAT access tube

In the following drawing, the dimensions of the probe PICO-T3PN, the spacers and the TECANAT access tube can be seen. Possible are maximum 4 segments PICO-T3PN at 1 meter tube length, beginning with the first segment direct at the soil surface.

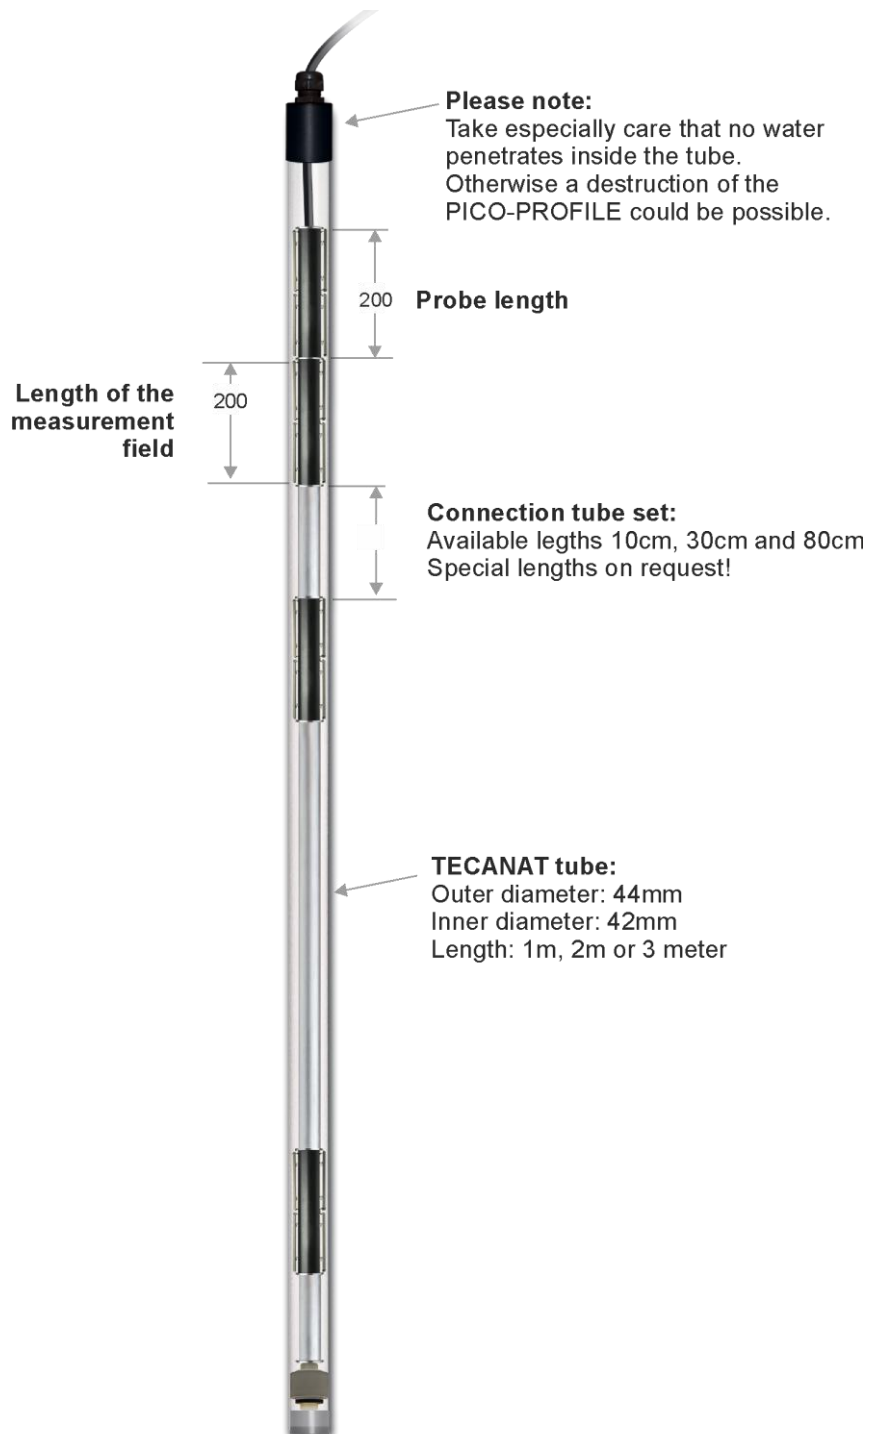


2.2 How to connect PICO-T3PN with connection tube set


Connection tube sets are available in 10cm, 30cm and 80cm.

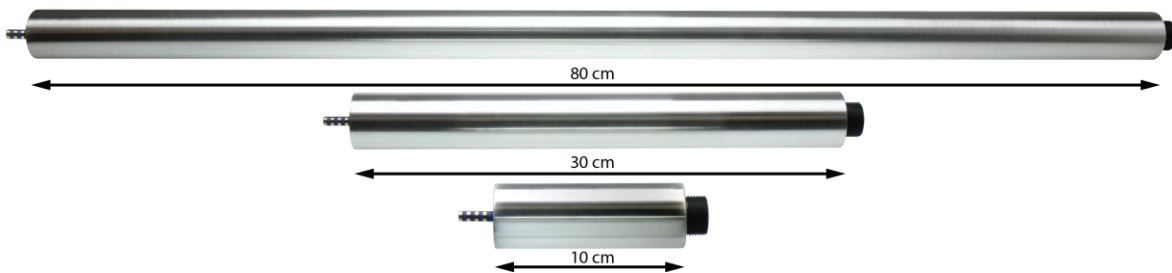

The measuring segment PICO-PROFILE T3PN is easy to connect with the connection tube set by screwing.

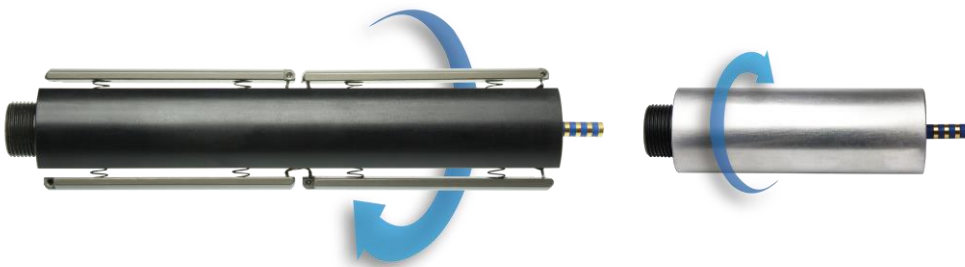


2.3 PICO DataLogger cable 5m or 15m length

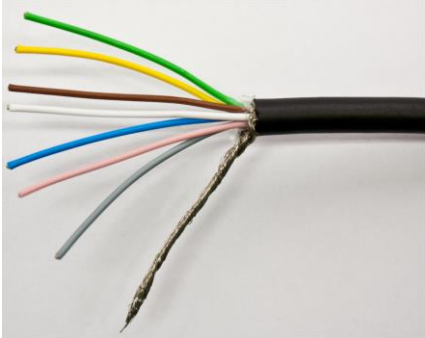
Wiring:		
Blank:	Shield	
Yellow:	COM (IMP-Bus)	
Grey:	R/T (IMP-Bus)	
Brown:	GND	
White:	+Vs (+12VDC)	
Blue:	RS485B or SDI12 Data	
Pink:	RS485A	

2.4 PICO DataLogger cable 25m, 50m or 100m length

For longer cable length it is necessary to use another cable:

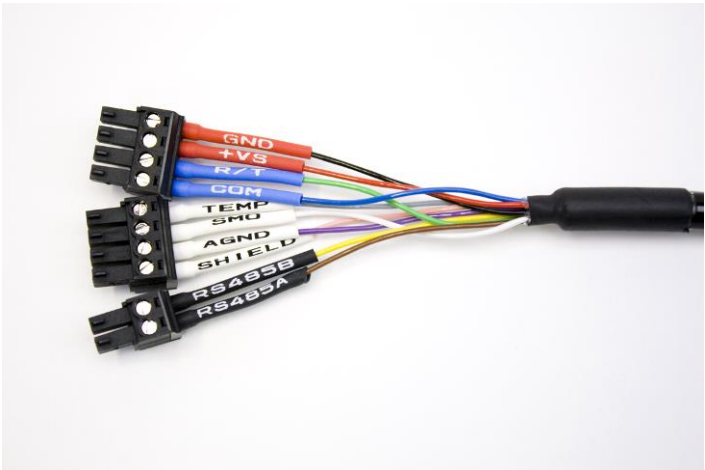
Wiring:		
Pink:	Shield	
Grey:		
Violet:		
White:		
Blue:	COM (IMP-Bus)	
Green:	R/T (IMP-Bus)	
Black:	GND	
Red:	+Vs (+12VDC)	
Yellow:	RS485B or SDI12 Data	
Brown:	RS485A	

2.5 PICO IMP-Bus cable 5m, 4-pin female connector (Item no.: 300115)

Pin layout:		
Pin 1:	+Vs (+12VDC)	
Pin 2:	R/T (IMP-Bus)	
Pin 3:	GND	
Pin 4:	COM (IMP-Bus)	
List of abbreviations:		
+Vs: + Voltage supply (12V/DC)	COM: Common (ground for IMP-Bus)	
GND: Ground (for voltage supply)	R/T: Receive/Transmit (on IMP-Bus)	


2.6 Accessories - SM-USB (Converter Module), (Item no.: 100020)

For connecting of the TRIME PICO-PROFILE (see 3.1 to 3.3, for 3.2 & 3.3 adapter required) via the USB-Interface to a PC. The module offers 2 Sensor-Interfaces, IMP-Bus (IMKO specific) and RS485 (industrial standard). One sensor can be powered out of the USB-Interface, if multiple sensors are connected external power supply is required!

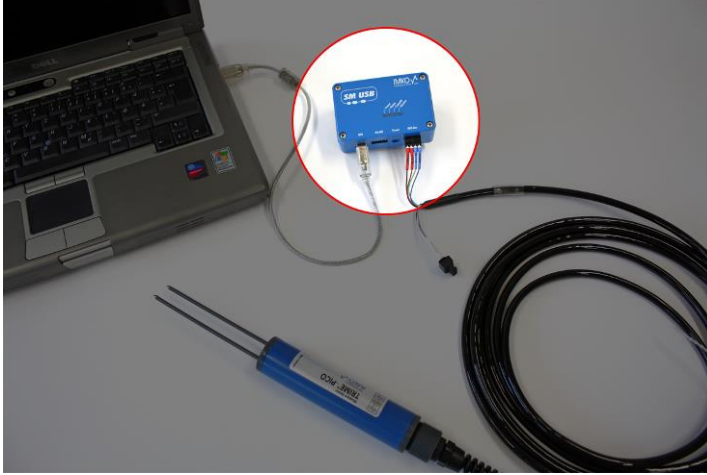

3 Access Tubes and Augers

The penetration depth of the measurement field of the 44mm TRIME tube-access-probe is up to 100mm into the soil. The measurement sensitivity is the highest near the access tube and decreases exponentially into the medium. Therefore the insertion method of the access tube is very important.

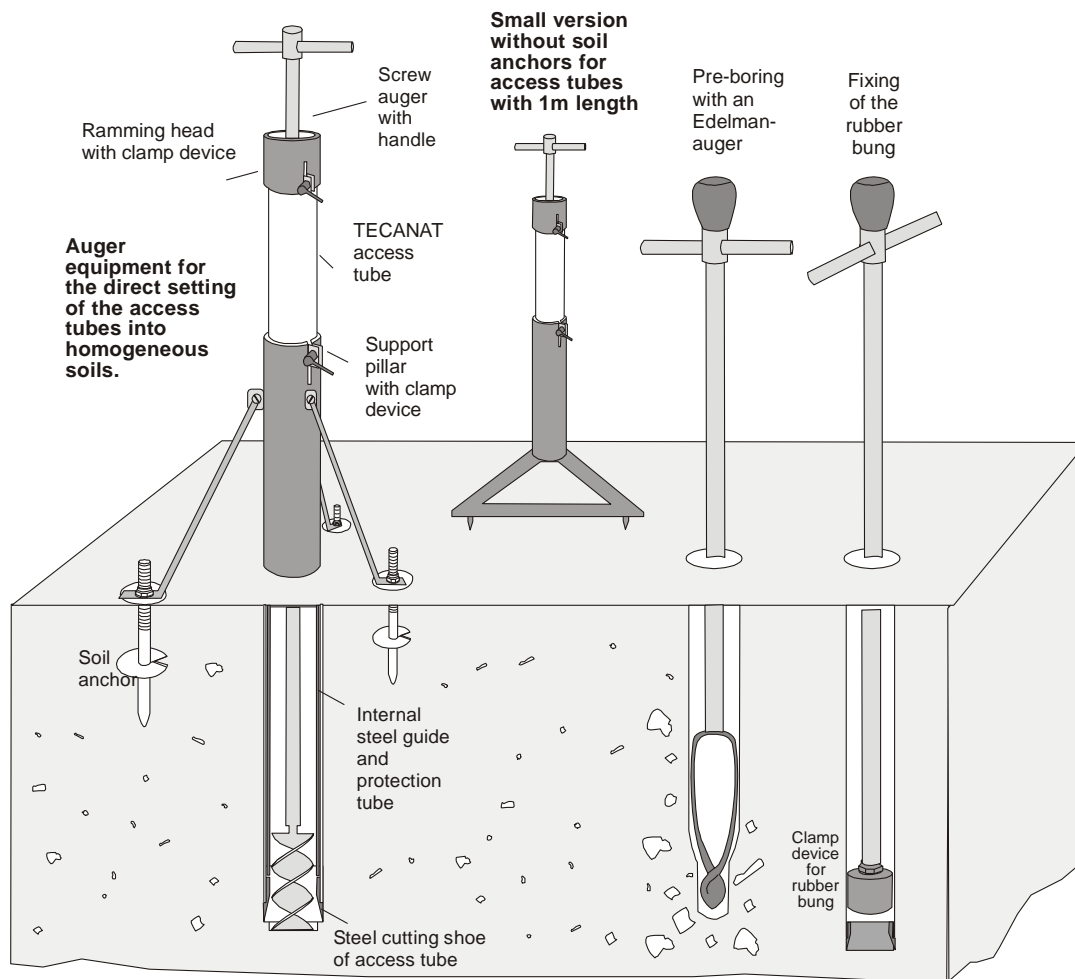


Pre-boring of bore holes with standard augers destroy the soil texture, because it is difficult to come to a good and close contact of the access tube inside the soil. With the described auger equipment it is possible to set the access tubes directly into homogenous soils without pre-boring. In very stony soils it is not possible to use this method. Therefore it could be possible to use an Edelman-Auger for pre-boring and closing the air gaps with mud. Changes in soil structure, and a delay time (up to 4 weeks) before it is possible to come to precise measurement values must then be accepted.

The IMKO auger equipment consists of: access tube support pillar with three soil anchors, ramming head with clamp device, screw auger with handle, clamp device for the rubber bung, and an internal steel guide/protection tube. Deliverable is a small version without soil anchors for setting of glass fibre tubes with 1m length.

A steel cutting shoe is glued into the access tube. The screw auger, that moves easily within the guide tube is used to drill out soil to about 0,1m below the cutting shoe. Depending on soil homogeneity, the tube can be hammered 5..10cm into the soil. This cycle is repeated until the tube is fully installed. The internal protection tube is then removed and the access tube can be sealed by a rubber bung.

3.1 Instructions for Access Tube Installation

The following instructions should be taken account of:

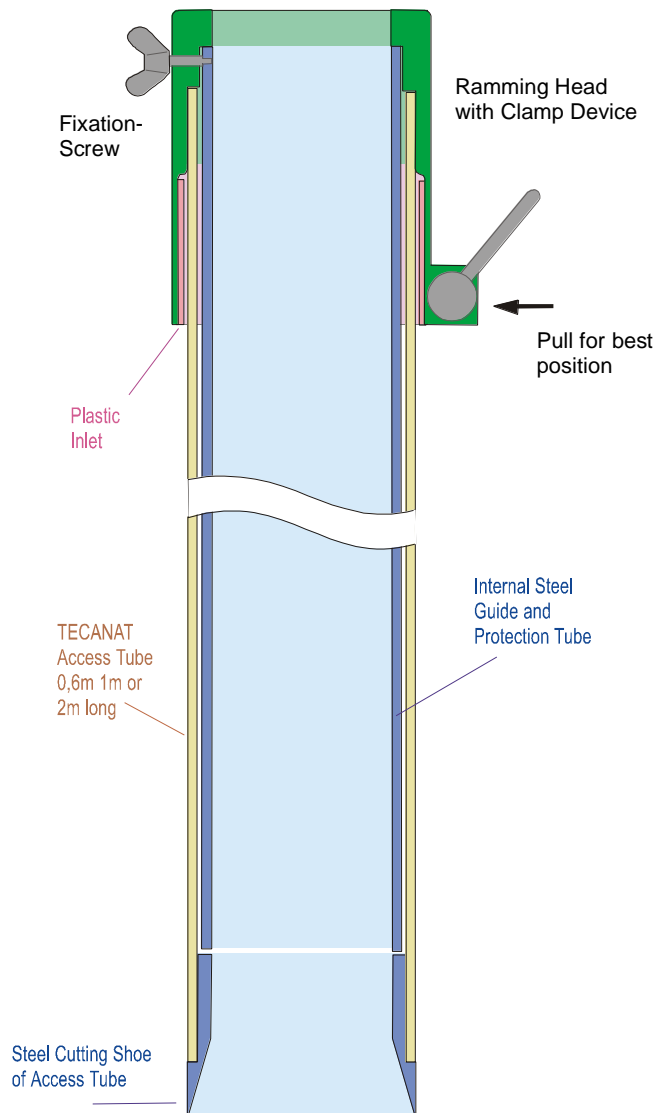

The ramming head, the TECANAT access tube and the internal steel guide and protection tube are one unit.

The internal protection tube has to lie on the cutting shoe of the access tube, before it can be fixed with a screw to the ramming head. This fixation is necessary to secure the shoe against being squeezed out by the returning force of the hammer-blow.

The access tube, however, is fixed to the ramming head by the clamp device. Both fixation screw and clamp device should be controlled during the installation process and be re-adjusted with the adjustable levers if necessary.

The screw auger that moves easily within the guide tube is used to drill out soil to about 0,1m below the cutting shoe. Depending on soil homogeneity, the tube is then hammered 5-10 cm into the soil with a plastic hammer (with open support pillar clamps!). The guide tube is not used for making the hole in the first instance because this could result in soil compaction around the hole, which would lead to higher measurement values.

The access tube support pillar with three ground anchors avoids vibrations that would cause air gaps. Then the clamp of the support pillar must be closed and the soil can be removed with the screw auger. When the tube reach the support pillar, it must be removed and the access tube can be inserted to the final depth without the support pillar.

A plastic collar should be mounted around the tube to prevent water from running down the tube wall and a plastic cap to protect the tube against rain.

3.2 Inserting and Fixing the Rubber Bung

1. Orient the rubber bung with the black rubber **washer downwards**.
2. Insert the rubber bung into the TECANAT tube.
3. Let it glide down or push to the bottom of the tube.



4. Fix the rubber bung with the screwing adaptor.



The rubber bung can be pushed into the access tube with the screw- adaptor and the handle (the screw-adaptor can be replaced instead of the screw auger) and can be fixed at the bottom of the access tube with two turns of the handle. If pushing down the rubber bung turns out to be difficult, just apply some talcum powder on the rubber bung sides and into the access tube.

3.3 Instructions for Water Proof Installation

Attention! Risk of Distruction!

The TECANAT tube is made of highly water resistant material in order to warrant for a long life-span of the tube and the installed PICO-PROFILE probe. In spite of the robust construction, it is to ensure that no water can penetrate into the TECANAT tube. The rubber bang has to be installed correctly and the tube head has to be sealed very secure against water ingress.

Any damage caused by faulty installation is not covered by the warranty!

4 Remote Power Supply to TRIME PICO-PROFILE

The operation of TRIME sensors may cause problems when power has to be supplied via long cables. There are limitations to the maximum cable length depending on the cable diameter.

When power is supplied over long distance the maximum cable length depends on the cable cross section **A**, the supply voltage **V_s** and the number **n** of the sensors measuring simultaneously. Device-specific data also be applied to the formula:

Power consumption during measurements:	$I_{norm} = 100\text{mA @ } 12\text{V/DC}$
Power consumption at min. voltage:	$I_{max} = 175\text{mA @ } 7\text{V/DC}$
Supply voltage:	$V_s = 12\text{V}$
Minimum sensor voltage at circuit end:	$V_{min} = 7\text{V}$
Wire cross section:	$A = 0,34\text{mm}^2$
Specific electrical resistance of copper:	$\rho = 0.0178\Omega \times \text{mm}^2 / \text{m}$
Number of sensors:	$n = 1\dots$

The maximum possible circuit length l_{max} can then be calculated in the following manner:

$$l_{max} = \frac{A \cdot (V_s - V_{min})}{2 \cdot \rho \cdot n \cdot I_{max}}$$

Please see the following the following example:

In the IMP232 environmental measurement system a bus cable with a wire cross section of $A = 0.34 \text{ mm}^2$ is normally used. We further assume that the power supply voltage is $V_s = 12 \text{ V}$ and only one sensor is designated to measure. Thus $n = 1$.

$$l_{max} = \frac{0.34\text{mm}^2 \cdot (12\text{V} - 7\text{V})}{0.0356\Omega \frac{\text{mm}^2}{\text{m}} \cdot 1 \cdot 0.175\text{A}} = 270\text{m}$$

In the above calculation, no tolerance is included; for security reasons the calculated cable length should be reduced by 10% to obtain a realistic value.

In order to increase the maximum possible cable length several solutions are feasible.

- Using cables with larger conductor diameters
By using 6-core conductor cables instead of 4-core, the cable length can be doubled as two extra cores can be used for power supply. Cables with conductors of larger diameters will further increase the maximum cable length possible.
- Increasing the power supply voltage
Power supply voltage can be increased up to 17V, thereby raising the maximum length from 270m to 540m in the example calculation above.
- Installation of buffer batteries in the distributor
Additional storage batteries close to the TRIME sensors, e.g. in the distributor, allow cable lengths up to 1km and enable simultaneous measurement of several sensors. However, this method requires an additional charging circuit for the buffer storage battery.
- Installation of a voltage regulator at the distributor
Voltage loss in the cable can be reduced with a 30V power supply and an installation of a voltage regulator directly in front of the TRIME sensor, thus allowing circuit lengths of up to 1km.

Which solution is best suited mainly depends on the nature of the power supply of the measurement system:

- ▶ **Battery supply:** solution 1 and possibly solution 3 should be considered, the latter being relatively expensive.
- ▶ **Mains supply:** solutions 1 and 2 could be combined, or, more expensive, solutions 2 or 4 could be chosen.

5 Datalogging configuration examples


PICO probes offer the possibility to use three different options for serial communication:

- The robust and secure (opto-isolated) IMP-Bus for large area monitoring networks with cable length >500 meter,
- the RS485 as an international standard serial interface for connection of PICO probes to standard PC's, PDA's and other computers,
- or the SDI12 interface for direct connection to SDI12 dataloggers.

5.1 PICO probes connected to the GlobeLog data logger via the IMP-Bus




- Up to 48 TRIME® PICO probes are connectable
- **Large area monitoring with cable length up to 500 meter via IMKO's robust and secure IMP-Bus**
- 2 MByte data storage capacity
- **Data transfer via cellular radio**
- Robust, lightweight, weatherproof (IP67)
- Easy programming
- Low Power
- Distribution modules with 3, 6 or 12 connectors

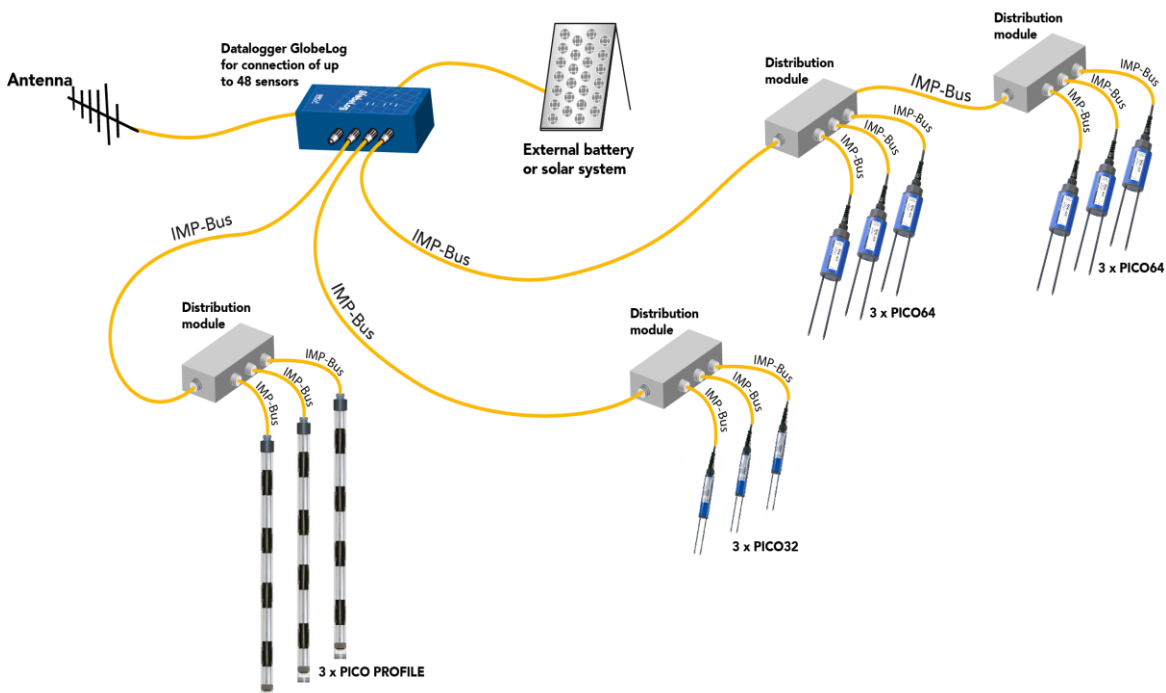

5.2 PICO probes connected to a PC under Windows


With IMKO's small software package TRIME WIN-MONITOR (cost free) it is possible to collect measurement data from up to 60 PICO probes to a PC. TRIME WIN-MONITOR runs under Windows. With the software PICO-CONFIG it is possible to configurate single PICO probes, e.g. to select a special calibration curve inside the PICO probe. The connection to the PC can be configured via the module SM-USB and a USB-port to the PC.

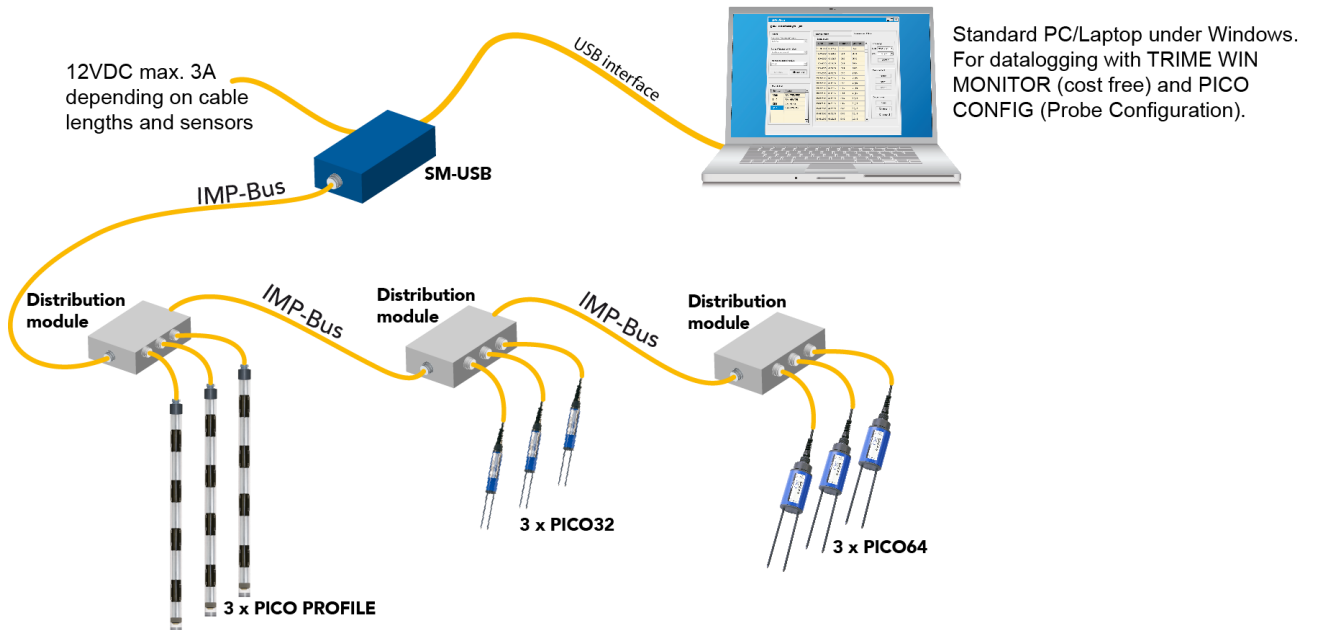

5.3 PICO probes connected to SDI12 dataloggers

SDI12 is a serial 1-wire interface for simple and easily connection of intelligent sensors to SDI12 dataloggers. Except to the 1-wire data line there are only 2 further cables necessary for power supply. Up to 10 SDI12 sensors can be connected to the SDI12 interface.

Please note: The SDI12 cable length is limited. For large area monitoring networks with cable length up to 500 meter we recommend to use IMKO's robust and secure IMP-Bus with opto-isolated (galvanic isolated) transmission signals.

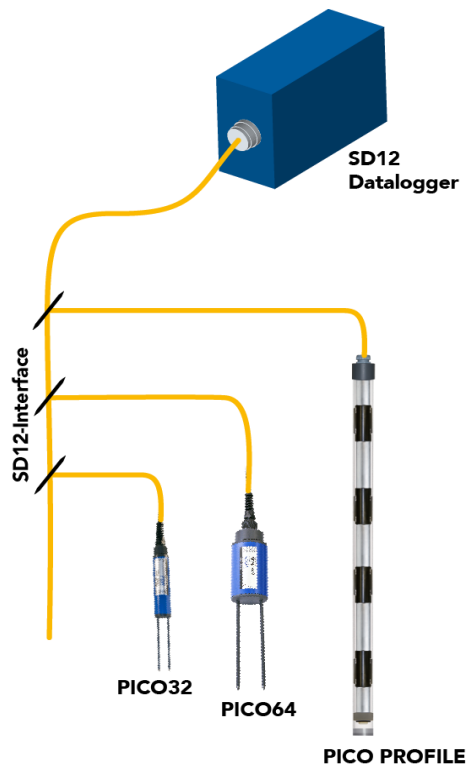

6 Information on Lightning Protection of a Sensor Network *(IMP-Bus, GlobeLog Logger and integrated Sensors)*

6.1 Introduction

Lightning strikes can cause considerable and costly damage to unprotected electronics. The equipment is often totally destroyed. A good number of users are not or only partially insured. Customers who have lightning protection insurance must comply with defined clauses regarding lightning and excess voltage. Insurance companies only cover the damage when compliance with the defined clauses has been proven. IMKO strongly recommends adequate lightning / excess voltage protection equipment for environmental measurement systems.

6.2 Excess voltage protection on 110/220V mains supply

Lightning strikes in proximity to high-voltage transmission lines can cause excess voltage in the mains power supply which may result in damage of electronic components. Environmental measurement systems with 110/220V mains supply are at risk from this excess voltage. It may affect the whole system through the power supply unit and the central station (GlobeLog Logger or SM-USB). Excess voltage can even enter the measuring system through the data acquisition computer's mains power supply. An excess voltage protection is highly recommended for all 110/220V devices connected to a sensor system

6.3 Protection of modem and telephone lines

Telephone lines are at risk from excess voltage. If a modem is connected to the measurement system the telephone line should also be protected by a lightning protection module.

6.4 Excess voltage protection for network modules by "SM-Blitz"

Excess voltage caused by lightning strokes in close proximity to the environmental measurement test system may enter the IMP-Bus transmission lines. Longer lines increase the risk of lightning strikes. Theoretically maximum protection is achieved by installation of a lightning protection module (SM-Blitz) in front of each SM-Module. Lightning protection is not cheap but it is certainly worthwhile. A compromise should be found between costs and the maximum-affordable protection, i.e. interconnection of adjacent SM-Modules to lightning protected groups.

6.5 Lightning protection on meteorological towers

SM-Modules installed on meteorological towers cannot be protected from lightning strikes. The field strength resulting from the electromagnetic fields and the associated accumulated energy will cause damage to the electronics. Two solutions to the problem:

- ▶ Erect a higher lightning conductor close to the meteorological tower serving as a lightning conductor.
- ▶ Install the measuring modules a number of metres away. Then all lines coming from the tower have to be protected by lightning protection modules.

6.6 Installation instructions for SM BLITZ lightning protection modules

Basically, there are two potential sources of risk in the field of environmental measurement technology: transmission lines and sensors or network devices. Lightning protection modules should always be installed at the beginning and at the end of a circuit in order to protect the electronics from excess voltage (Attention: SM-Blitz modules have a protected and an unprotected side).

The SM-BLITZ lightning protection module has to be grounded using a ground conductor with a wire cross-section of at least 6 mm² screwed to the long side of the module. A 2-metre long grounding rod may serve as a ground conductor. Grounding is optimal when the grounding rod is in direct contact with ground water.

6.7 Conclusion

Only limited protection against excess voltage is possible where natural phenomenon such as lightning strikes are concerned. Direct lightning strikes may cause damage nevertheless.

If you have any questions regarding lightning protection please do not hesitate to contact us.

Tel.: 0049 - (0)7243 - 5921-0

Fax: 0049 - (0)7243 – 90856

e-mail: info@imko.de

7 TRIME PICO-T3PN theory

7.1 Introduction

The measuring of soil water content with Time Domain Reflectometry is now a well established method. However water content profiling is not possible with conventional TDR rod probes. The TRIME tube probe was developed for this reason.

Since 1994 the TRIME-T3 has found numerous applications in earth and environmental sciences, fulfilling even the most exacting requirements.

7.2 Measuring Field

The effective penetration depth of the probe is about 10 cm with the highest sensitivity in the immediate vicinity of the access tube and decreases exponentially with distance. Figure 1 shows the electric field distribution of the probe and the approximate measuring volume.

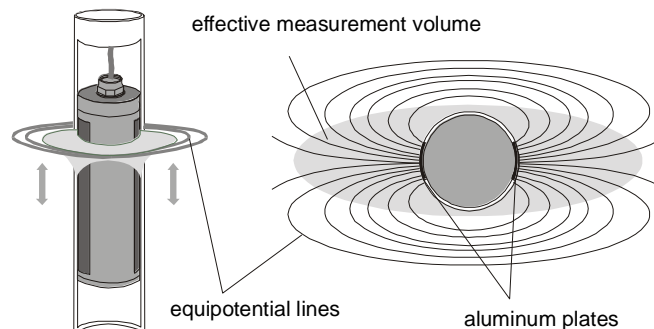


Figure 1: Electric field distribution of the TRIME probe and approximate measuring volume.

Note that the necessity of a close contact between access tube and material is vital for reliable measurements and that the tubes should be installed by our recommended method.

For example at an assumed water content of 15 vol. % an air gap of 1 mm around the whole length of the tube would result in an underestimation of 1 - 2 vol. %.

At a water content of 25 vol. % the error would be 5 vol.-% with an air gap around the tube.

At very high water contents (50 vol. %) errors may reach 10 vol. % with an air gap around the tube.

In the case of a water filled gap under conditions of saturation the gap error would be much smaller.

Problems may arise, however, in very inhomogeneous soils and when drilling under very dry conditions. For these soils other drilling methods are recommended (e. g. pre-boring with an Edelman auger, washing mud into the cavity around the tube). Losses in accuracy must then be accepted, and measurements immediately after installation are not recommended.

Problems can also arise in swelling and shrinking soils, since cracks develop especially along the access tubes.

7.3 Measuring experiences

The new TRIME technique was thoroughly tested in the field and compared both to neutron probe measurements and thermo gravimetrically determined values.

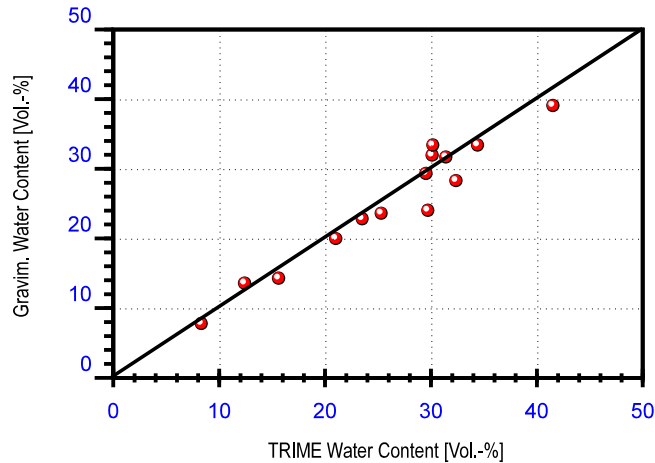


Figure 2: Comparison of TRIME measurements and gravimetric water content determination for a clayey soil.

7.4 Summary

The TRIME tube probe is a promising new tool for determining water content profiles with the TDR method. Fast, routine and non destructive measurements of water content without the use of hazardous radioactive materials are possible. A measuring accuracy of ± 2 vol.-% is possible, provided that soil and access tube are in close contact and bulk soil electrical conductivity doesn't exceed 2 dS/m.

8 Basic Calibration with the Calibration Set

8.1 What is a basic calibration?

Basic calibration serves to compensate the cable length and tolerances of the probe mechanics (thickness of the rod coating, rod length, etc.). After two measurements, one in dry and one in water-saturated glass beads, the calibration data is calculated and stored in the TRIME sensor.

Every TRIME PICO-PROFILE sensor must be calibrated before it can supply proper measurement results. **Basic calibration is carried out by IMKO in the factory prior to shipment.**

8.2 What are the benefits of the calibration set for the user?

With the calibration set you can easily carry out basic calibration of your TRIME sensor yourself.

- ▶ If defective probe rods must be changed, you can perform the required basic calibration yourself.

The calibration set **cannot** be used for establishing a material (soil) specific calibration. For this purpose a measurement dataset must be created for the specific material. The complementary calibration program **TRIME-Tool** is required to calculate the calibration data for this dataset and to download it to the TRIME PICO-PROFILE-Probe.

8.2.1 Calibration set for TRIME probes

For basic calibration of TRIME probes.

- 2 x boxes (7 litres.)
- 22kg glass beads

Item no.: 305017



8.3 How to perform a basic calibration?

8.3.1 Preparation of the glass beads

The glass beads, supplied with the calibration set, have to be prepared first:

Fill up one bucket until the rods of the probe can be immersed completely. To obtain a consistent density, knock the bucket on the ground several times.

- ▶ The density of the glass beads increases with frequent insertion of probes. Therefore the glass beads should be poured out into another bucket and poured back to achieve the original density.

Now the second bucket has to be filled with water in order to be able to fill in the glass beads without leaving air-bubbles. An additional precaution against air-bubbles is to stir slightly while filling in the glass beads. The container must now be knocked on the ground several times to obtain a consistent density. The surplus water must be poured out until the depth of the water film above the glass beads is less than 2mm.

The water-saturated glass beads should be in a temperature range between 20°C and 25°.

- ▶ **Attention:** Water dissolves Na_2O and K_2O from glass which causes a rising pH-value and higher electrical conductivity. **New glass beads have to be washed intensively with tap water!!!**

1. Fill a bucket with water
2. Stir the beads under water to drive out all air bubbles
3. Pour out the water. This procedure should be done with new glass beads at least five times, each time with fresh water. If the glass beads have been in use for a prolonged period, three times is sufficient.

Please note that the electrical conductivity of the water-saturated glass beads medium increases already after a few days storage. Therefore the glass beads must be washed again before the next calibration.

8.3.2 Basic calibration procedure

Basic calibration must be performed using the calibration program *Pico-Config*. Please read the information about basic calibration with *Pico-Config* in **chapter 12** of this document.



Fig.: PICO T3 probe head inserted in a TECANAT calibration tube which again is installed in dry glass beads. Make sure that the tube probe's wave guides are completely inserted into the glass beads when measuring. The basic alignment will fail if the wave guides are in part surrounded by air.

8.3.3 Material specific calibration

Your TRIME measuring system operates with a universal calibration for mineral soils as a standard.

The following parameters limit the application range of the universal calibration:

- *Clay content:* >50%
- *Organic content:* >10%
- *Bulk density:* <1.1kg/dm³ or >1.7kg/dm³

Exceeding these limits may cause the tolerances given on page 5 to be overstepped.

Material-specific calibration is advisable if your soil is listed above or if you require accuracy down to the last digit. The **PICO-CONFIG** software is required for setting up a material-specific calibration (*download under www.imko.de*).

A test series with reference values is necessary for performing material-specific calibration (e.g. *Oven drying at 105°C until weight is constant*). The test series –and consequently the calibration– should include minimum and maximum moisture values. TRIME readings and reference values are compared in a table. The calibration coefficients must then be calculated and uploaded to the TRIME-device.

9 TRIME WIN MONITOR

9.1 Installation

Download the file *Trime_WinMonitor x.xxx.zip* to the PC from IMKO website. Unzip the files *Trime_WinMonitor_Setup.msi* and *Setup.exe* from *Trime_WinMonitor x.xxx.zip*.

Double-click *Trime_WinMonitor_Setup.msi* and follow the instructions to install the software. After the installation, Trime_WinMonitor should be seen on Start->Program menu and Desktop.

1 how to use

9.2 Connect Trime-PICO to a PC

If Trime-PICO is tested, it can be connected to a PC via RS485 bus or the IMP Bus with a the SM-USB module. Several Trime-PICO probes may be netted and tested on IMP bus or RS485.

9.3 Operating the program

Start the program.

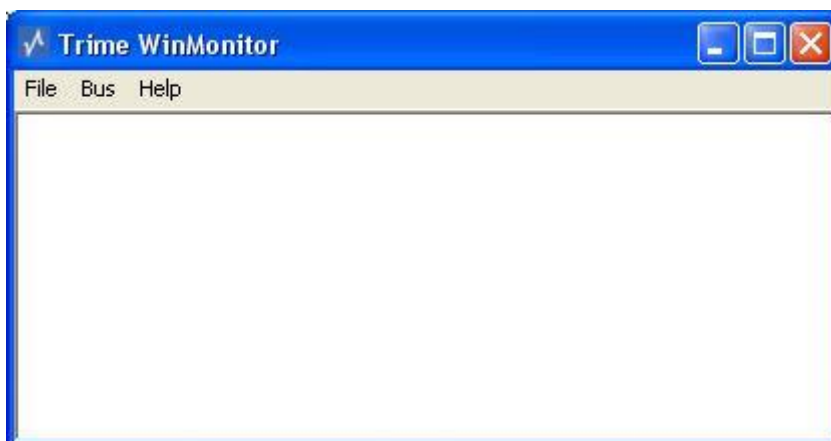


Fig. main menu

Click **Configuration** from the menu **Bus**

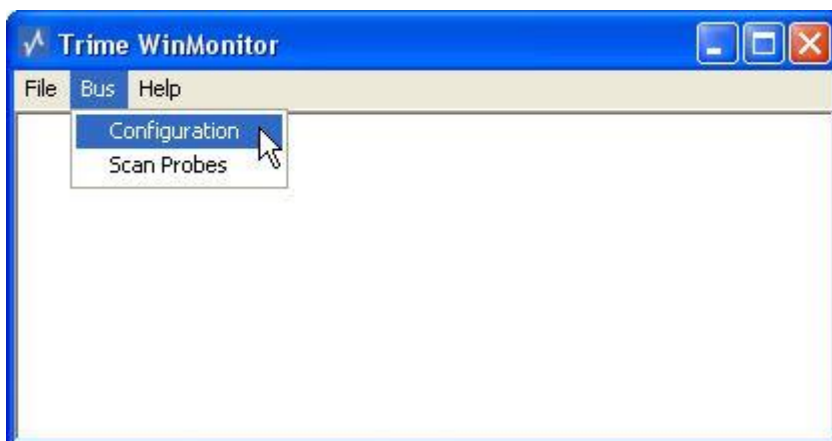


Fig. enter Configuration

In the dialog **Configuration** (Fig.2.3) the parameters can be selected: **SerialPort: Use the selected port or Automatically search the port**, **Baudrate** (default value 9600), **Scanned Trime-FM, IT, EZ, IPH, ES with Station Number** (1-250) or **Scanned Trime-Pico with Serial Number**(30000-99999).

For the parameter **SerialPort**, only the option **Use the selected port** can be used if the probe is Trime-FM,IT,ET,IPH,ES. The both options for Trime-Pico.

In the field **Scanned Trime-FM, IT, EZ, IPH, ES with Station Number** the station numbers of a TRIME sensor can be preset and in the field **Scanned Trime-Pico with Serial Number** the serial numbers of a Trime-Pico which are integrated in an IMP-bus network.

Click **OK** to save the changes of parameters to the configuration file **TRIME WinMonitor.con**.

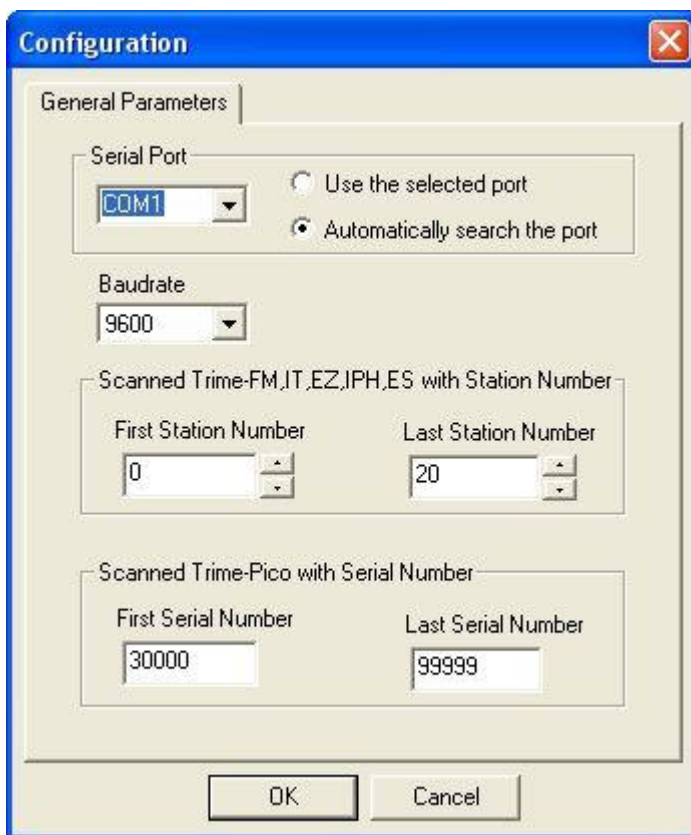


Fig. Configuration

Click **Scan Probes** to scan the connected probes.

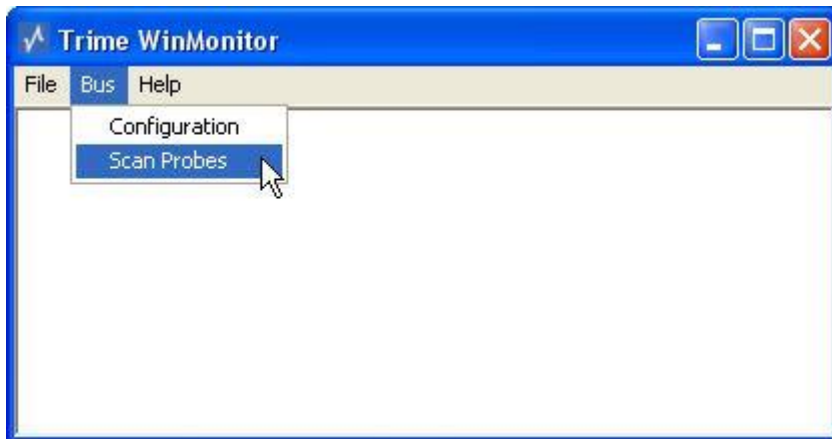


Fig. enter Scan Probes

The **Progress Dialog** will be shown for several seconds.



Fig. progress for scanning

The dialog **Probe List and Measure** is entered.

- a. The basic data of the scanned probe is listed in the upper list. For example, two Trime-Pico probes are in the list.
- b. Basically two functions, **Single Measure** and **Circle Measure**, and one adjustment, **Dry Density**, are provided in this dialog.

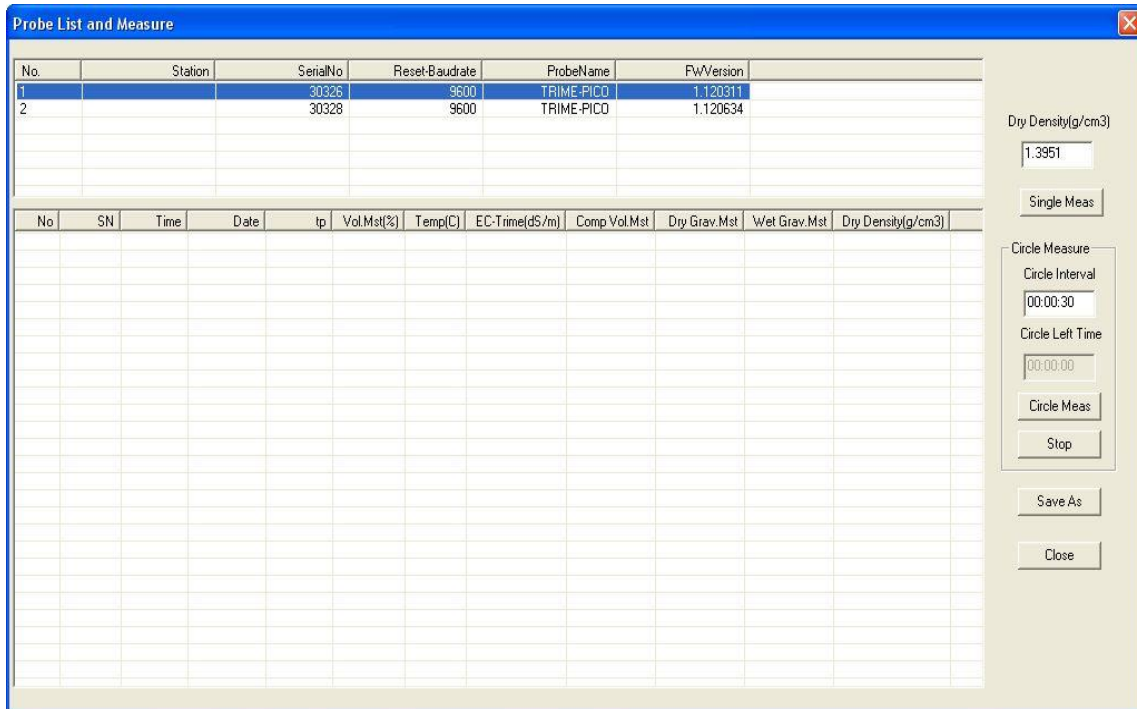


Fig. Probe List

Single Measure

- a. Click button **Single Meas** to measure only one time
- b. The **Progress Dialog** will be shown for several seconds. It lasts maximal 15 seconds for Trime with a station number or maximal 5 seconds for Trime-Pico.

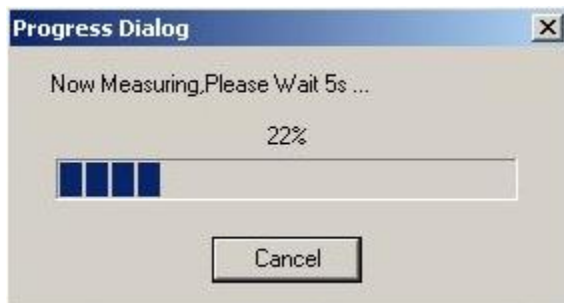


Fig. progress for measuring

- c. The reading is displayed in the lower list (Fig.2.8). The SN, tp and temperature values aren't displayed for Trime with the station number. All measuring data is automatically saved in the file **Monitor+SerialNum.asc** separately on the same path as **Trime WinMonitor.exe**. For example, the data in Fig. is stored in the file **Monitor30326.asc** with the records of SN30326 and **Monitor30328.asc** of SN30328. When the measurement is carried out next time, the data will be appended in the same file. That is, one probe corresponds to one file.

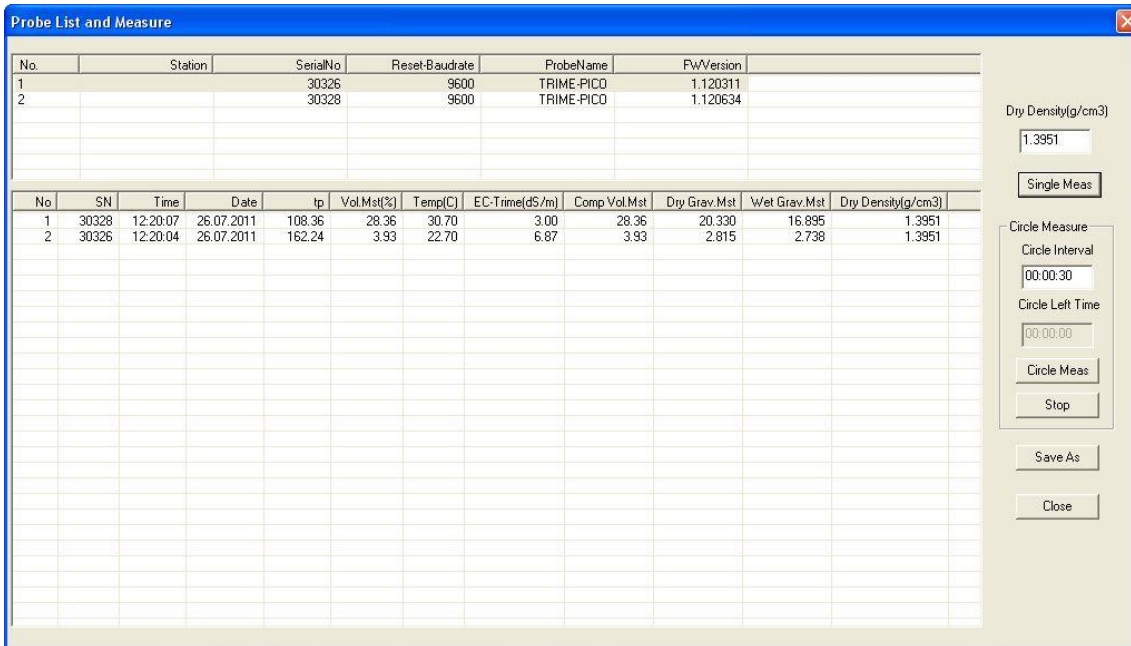


Fig. single measure

- d. Click button **Save As** to enter the dialog **Save** to save the data to a file which may be new or already existing. If selecting an existing file, the data will be appended. If several Trime-Pico probes are on the bus, all the data are saved in the file together.

2. Circle Measure

- a. Put in the interval (>23s for Trime and >10s for one Trime-Pico) in **Circle Interval**. The format must be hh:mm:ss (Fig.). If several Trime-Pico probes are on the bus, the interval should be bigger than 10xprobe number. For example, there are 3 Trime-Pico probes on the bus, the interval should be minimal 30 seconds.
- b.

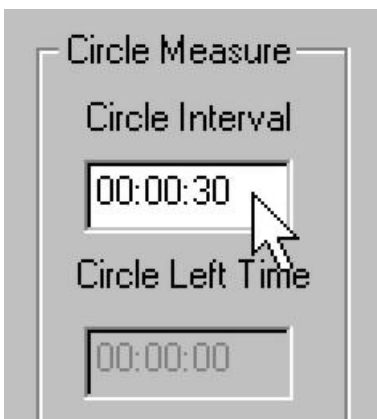


Fig. set circle interval

- c. Click button **Circle Meas** to measure periodically.
- d. In **Circle Left Time** update the time until the next measurement is carried out. This time is approximate.
- e. The readings are displayed in the lower list (Fig. 2.10) and have automatically been saved in the file **Monitor+SerialNum.asc** on the same path as **Trime WinMonitor.exe**. Refer to the step 4.c.

Probe List and Measure

No.	Station	SerialNo	Reset-Baudrate	ProbeName	FWVersion
1		30326	9600	TRIME-PICO	1.120311
2		30328	9600	TRIME-PICO	1.120634

No	SN	Time	Date	tp	Vol.Mst(%)	Temp(C)	EC-Time(dS/m)	Comp.Vol.Mst	Dry Grav.Mst	Wet Grav.Mst	Dry Density(g/cm3)
1	30328	12:25:20	26.07.2011	108.79	28.79	30.70	3.00	28.79	20.640	17.109	1.3951
2	30326	12:25:16	26.07.2011	162.14	3.92	23.00	6.86	3.92	2.812	2.735	1.3951
3	30328	12:24:50	26.07.2011	106.64	26.64	30.70	2.89	26.65	19.099	16.036	1.3951
4	30326	12:24:46	26.07.2011	162.26	3.93	23.00	6.86	3.93	2.816	2.739	1.3951
5	30328	12:24:20	26.07.2011	106.64	26.64	30.70	2.89	26.65	19.099	16.036	1.3951
6	30326	12:24:16	26.07.2011	162.22	3.93	22.90	6.86	3.93	2.815	2.738	1.3951
7	30328	12:23:50	26.07.2011	108.73	28.73	30.70	3.00	28.73	20.594	17.077	1.3951
8	30326	12:23:46	26.07.2011	162.27	3.93	23.00	6.87	3.93	2.817	2.740	1.3951
9	30328	12:23:20	26.07.2011	106.20	26.20	31.00	2.89	26.20	18.781	15.811	1.3951
10	30326	12:23:16	26.07.2011	162.27	3.93	22.90	6.87	3.93	2.817	2.740	1.3951
11	30328	12:22:50	26.07.2011	107.92	27.92	30.70	3.00	27.92	20.013	16.675	1.3951
12	30326	12:22:46	26.07.2011	162.09	3.92	22.70	6.87	3.92	2.810	2.733	1.3951
13	30328	12:22:20	26.07.2011	107.22	27.22	31.00	3.00	27.22	19.511	16.325	1.3951
14	30326	12:22:16	26.07.2011	162.18	3.92	22.70	6.87	3.92	2.813	2.736	1.3951
15	30328	12:21:42	26.07.2011	107.99	27.99	30.70	3.00	27.99	20.065	16.712	1.3951
16	30326	12:21:39	26.07.2011	162.17	3.92	22.80	6.87	3.92	2.813	2.736	1.3951

Dry Density(g/cm3)
1.3951

Single Meas

Circle Measure
Circle Interval
00:00:30
Circle Left Time
00:00:26
Circle Meas
Stop
Save As
Close

Fig. the data list from near to far in chronological order

- f. Click button **Stop** to stop the circle measure.
- g. Click Button **Save As** to save the data as above explained at the step **4.d**.
- h. The data in Fig.2.10 is listed from near to far in chronological order. If the data from far to near is wanted, click the column title **Time**. The data will be shown as Fig. 2.11. If the data in the SN order is wanted, click the column title **SN**. The data will be shown as Fig. 2.12. If clicking the column title **Time**, the data will be shown again as Fig. 2.10.

Probe List and Measure

No.	Station	SerialNo	Reset-Baudrate	ProbeName	FWVersion
1		30326	9600	TRIME-PICO	1.120311
2		30328	9600	TRIME-PICO	1.120634

No	SN	Time	Date	tp	Vol.Mst(%)	Temp(C)	EC-Time(dS/m)	Comp.Vol.Mst	Dry Grav.Mst	Wet Grav.Mst	Dry Density(g/cm3)
16	30326	12:21:39	26.07.2011	162.17	3.92	22.80	6.87	3.92	2.813	2.736	1.3951
15	30328	12:21:42	26.07.2011	107.99	27.99	30.70	3.00	27.99	20.065	16.712	1.3951
14	30326	12:22:16	26.07.2011	162.18	3.92	22.70	6.87	3.92	2.813	2.736	1.3951
13	30328	12:22:20	26.07.2011	107.22	27.22	31.00	3.00	27.22	19.511	16.325	1.3951
12	30326	12:22:46	26.07.2011	162.09	3.92	22.70	6.87	3.92	2.810	2.733	1.3951
11	30328	12:22:50	26.07.2011	107.92	27.92	30.70	3.00	27.92	20.013	16.675	1.3951
10	30326	12:23:16	26.07.2011	162.27	3.93	22.90	6.87	3.93	2.817	2.740	1.3951
9	30328	12:23:20	26.07.2011	106.20	26.20	31.00	2.89	26.20	18.781	15.811	1.3951
8	30326	12:23:46	26.07.2011	162.27	3.93	23.00	6.87	3.93	2.817	2.740	1.3951
7	30328	12:23:50	26.07.2011	108.73	28.73	30.70	3.00	28.73	20.594	17.077	1.3951
6	30326	12:24:16	26.07.2011	162.22	3.93	22.90	6.86	3.93	2.815	2.738	1.3951
5	30328	12:24:20	26.07.2011	106.64	26.64	30.70	2.89	26.65	19.099	16.036	1.3951
4	30326	12:24:46	26.07.2011	162.26	3.93	23.00	6.86	3.93	2.816	2.739	1.3951
3	30328	12:24:50	26.07.2011	106.64	26.64	30.70	2.89	26.65	19.099	16.036	1.3951
2	30326	12:25:16	26.07.2011	162.14	3.92	23.00	6.86	3.92	2.812	2.735	1.3951
1	30328	12:25:20	26.07.2011	108.79	28.79	30.70	3.00	28.79	20.640	17.109	1.3951

Dry Density(g/cm3)
1.3951

Single Meas

Circle Measure
Circle Interval
00:00:30
Circle Left Time
00:00:26
Circle Meas
Stop
Save As
Close

Fig. the data list from far to near in chronological order

Probe List and Measure

No.	Station	SerialNo	Reset-Baudrate	ProbeName	FwVersion
1		30326	9600	TRIME-PICO	1.120311
2		30328	9600	TRIME-PICO	1.120634

No.	SN	Time	Date	tp	Vol.Mst(%)	Temp(C)	EC-Trime(dS/m)	Comp.Vol.Mst	Dry Grav.Mst	Wet Grav.Mst	Dry Density(g/cm3)
2	30326	12:25:16	26.07.2011	162.14	3.92	23.00	6.86	3.92	2.812	2.735	1.3951
4	30326	12:24:46	26.07.2011	162.26	3.93	23.00	6.86	3.93	2.816	2.739	1.3951
6	30326	12:24:16	26.07.2011	162.22	3.93	22.90	6.86	3.93	2.815	2.738	1.3951
8	30326	12:23:46	26.07.2011	162.27	3.93	23.00	6.87	3.93	2.817	2.740	1.3951
10	30326	12:23:16	26.07.2011	162.27	3.93	22.90	6.87	3.93	2.817	2.740	1.3951
12	30326	12:22:46	26.07.2011	162.09	3.92	22.70	6.87	3.92	2.810	2.733	1.3951
14	30326	12:22:16	26.07.2011	162.18	3.92	22.70	6.87	3.92	2.813	2.736	1.3951
16	30326	12:21:39	26.07.2011	162.17	3.92	22.80	6.87	3.92	2.813	2.736	1.3951
1	30328	12:25:20	26.07.2011	108.79	28.79	30.70	3.00	28.79	20.640	17.109	1.3951
3	30328	12:24:50	26.07.2011	106.64	26.64	30.70	2.89	26.65	19.099	16.036	1.3951
5	30328	12:24:20	26.07.2011	106.64	26.64	30.70	2.89	26.65	19.099	16.036	1.3951
7	30328	12:23:50	26.07.2011	108.73	28.73	30.70	3.00	28.73	20.594	17.077	1.3951
9	30328	12:23:20	26.07.2011	106.20	26.20	31.00	2.89	26.20	18.781	15.811	1.3951
11	30328	12:22:50	26.07.2011	107.92	27.92	30.70	3.00	27.92	20.013	16.675	1.3951
13	30328	12:22:20	26.07.2011	107.22	27.22	31.00	3.00	27.22	19.511	16.325	1.3951
15	30328	12:21:42	26.07.2011	107.99	27.99	30.70	3.00	27.99	20.065	16.712	1.3951

Dry Density(g/cm3): 1.3951

Single Meas

Circle Measure

Circle Interval: 00:00:30

Circle Left Time: 00:00:26

Circle Meas

Stop

Save As

Close

Fig. the data list in SN order

- i. Click button **Close** to close the dialog.

9.4 Explanation of measuring data

All the measuring data is listed in the list in Fig. Here explain the columns and their relationship.

tp: the pseudo running time(ps);

VolMst: the volumetric moisture to be measured by TDR principle;

TDRLevel: a TDR amplitude value which can be calibrated to electrical conductivity. It is displayed for Trime-FM,IT,ES,IPH,ES.

Temp(C): the material temperature(°C). It is only for Trime-Pico.

EC-Trime(dS/m): the electrical conductivity to be measured by Trime. It is only for Trime-Pico.

CompenVolMst(%): the volumetric moisture with the density compensation. It is calculated from VolMst and Dry Density with the equation [4] of chapter 3.

DryGravMst: the dry gravimetric moisture. It is calculated from CompenVolMst and Dry Density with the equation [5a] of chapter 3.

WetGravMst: the wet gravimetric moisture. It is calculated from DryGravMst with the equation [2c] of chapter 3.

DryDensity(g/cm3): the entered dry density.

9.5 File format

The file has the extension asc and is txt file. The columns are separated by the space.

1. The file format for Trime with station number (Trime-FM,IT,ES,IPH,ES) is shown in Fig. The columns in the file are Time, Date, VolMst(%), TDRLevel, CompenVolMst(%), DryGravMst(%), WetGravMst(%) and DryDensity(g/cm³).

Time	Date	VolMst(%)	TDRLevel	CompenVolMst(%)	DryGravMst(%)	WetGravMst(%)	DryDensity(g/cm ³)
10:11:29	26.07.2011	3.92	82.20	3.92	2.811	2.735	1.3951
10:12:09	26.07.2011	3.92	82.20	3.92	2.811	2.735	1.3951
10:12:39	26.07.2011	3.92	82.20	3.92	2.811	2.735	1.3951
10:13:09	26.07.2011	3.92	82.20	3.92	2.811	2.735	1.3951

Fig. the file format of Trime-FM,IT,ES,IPH,ES

2. The file format for Trime-Pico is shown in Fig.2.14. The columns in the file are SN, Time, Date, Tp, VolMst(%), Temp(C), EC-Trime(dS/m), CompenVolMst(%), DryGravMst(%), WetGravMst(%) and DryDensity(g/cm³).

SN	Time	Date	Tp	VolMst(%)	Temp(C)	EC-Trime(dS/m)	CompenVolMst(%)	DryGravMst(%)	WetGravMst(%)	DryDensity(g/cm ³)
30326	11:40:50	26.07.2011	162.13	3.92	22.20	6.87	3.92	2.811	2.735	1.3951
30326	12:14:21	26.07.2011	162.14	3.92	22.60	6.87	3.92	2.812	2.735	1.3951
30326	12:14:59	26.07.2011	162.23	3.93	22.60	6.87	3.93	2.815	2.738	1.3951
30326	12:15:29	26.07.2011	162.22	3.93	22.60	6.87	3.93	2.815	2.738	1.3951
30326	12:20:04	26.07.2011	162.24	3.93	22.70	6.87	3.93	2.815	2.738	1.3951
30326	12:21:39	26.07.2011	162.17	3.92	22.80	6.87	3.92	2.813	2.736	1.3951
30326	12:22:16	26.07.2011	162.18	3.92	22.70	6.87	3.92	2.813	2.736	1.3951

Fig. the file format of Trime-Pico

10 Quick guide for the Software PICO-CONFIG

10.1 Connection of the RS485 or the IMP-Bus to the SM-USB Module

The SM-USB provides the ability to connect a PICO probe either to the standard RS485 interface or to the IMP-Bus from IMKO, which enables the download of a new firmware to the PICO probe. Both connector ports are shown in the drawing below.

The SM-USB is signalling the status of power supply and the transmission signals with 4 LED's. When using a dual-USB connector on the PC, it is possible to use the power supply for the PICO probe directly from the USB port of the PC without the use of the external AC adapter.

Connection to the Probe:

RS485 Connector

0V GND

+Vs

RS485B

RS485A

+12VDC

IMP-Bus Connector


With the option to accomplish a download of the firmware for the PICO probe

0V GND

+Vs

R/T IMP-Bus

COM IMP-Bus

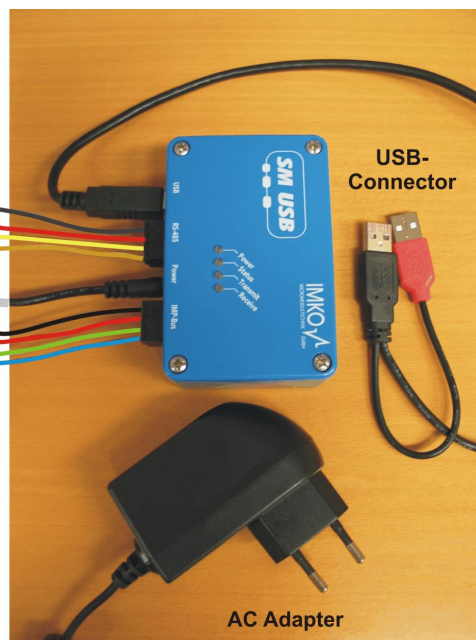

Please note: The PICO-PROFILE wiring and cabling has other colours!

How to start with the USB-Module SM-USB from IMKO


- Install USB-Driver from USB-Stick.
- Connect the SM-USB to the USB-Port of the PC and the installation will be accomplished automatically.
- Install Software **PICOConfig-Setup.msi** from USB-Stick.
- Connection of the PICO probe to the EX9531 via RS485A, RS485B and 0V.
- Check the setting of the COM-Ports in the Device-Manager und setup the specific COM-Port with the Baudrate of 9600 Baud in PICO-CONFIG with the button "**Bus**" and "**Configuration**" (COM1-COM15 is possible).
- Start "**Scan probes**" in PICOConfig.
- The PICO probe logs in the window „**Probe List**“ after max. 30 seconds with its serial number.

Note 1:

In the Device-Manager passes it as follows:

Control Panel → System → Hardware → Device-Manager



Under the entry “Ports (COM & LPT)” now the item “USB Serial Port (COMx)” is found.

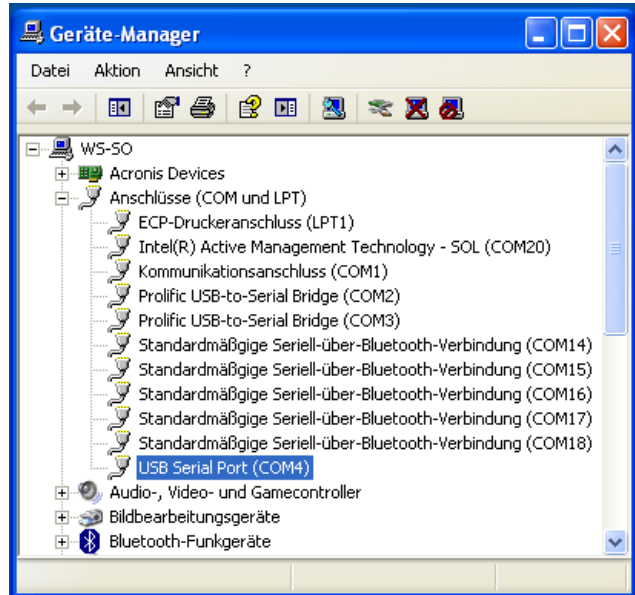

COMx set must be between COM1....COM9 and it should be ensured that there is no double occupancy of the interfaces.

If it comes to conflicts among the serial port or the USB-SM has been found in a higher COM-port, the COM port number can be adjusted manually:

By double clicking on "USB Serial Port" you can go into the properties menu, where you see "connection settings" – with "Advanced" button, the COM port number can be switched to a free number.

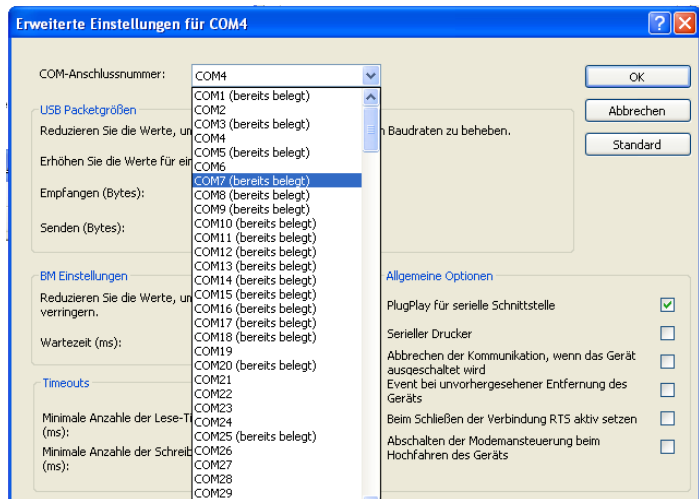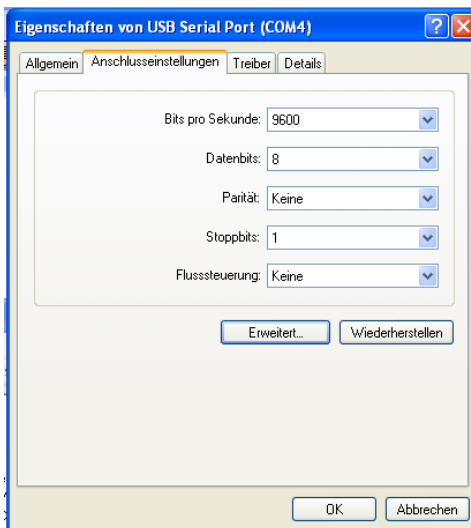


After changing the COMx port settings, PICO-CONFIG must be restarted.

10.2 Bus Configuration and Probe Scan

With PICO-CONFIG it is possible to make process-related adjustments of individual parameters of the PICO probe. Furthermore the measurement values of the PICO probe can be read from the probe via the RS485 or IMP-Bus interface and displayed on the screen.


In the menu "Bus" and the window "Configuration" the PC can be configured to an available COMx-port with the Baudrate of 9600 Baud.

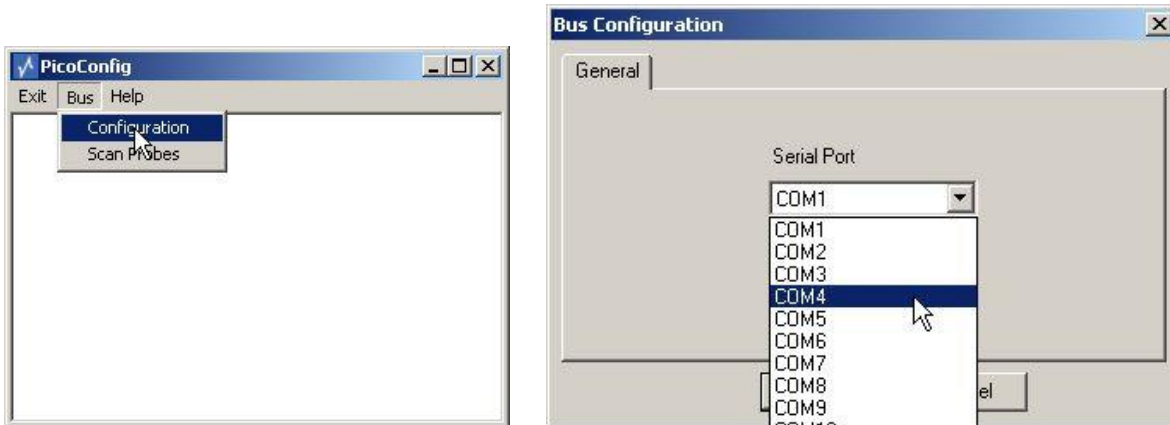

10.3 Scan of connected PICO probes on the serial interface


In the menu "Bus" and the window "Scan Probes" the RS485 bus can be scanned for attached PICO probes (takes max. 30 seconds).

PICO-CONFIG reports founded PICO probes with its serial number in the window "Probe List".

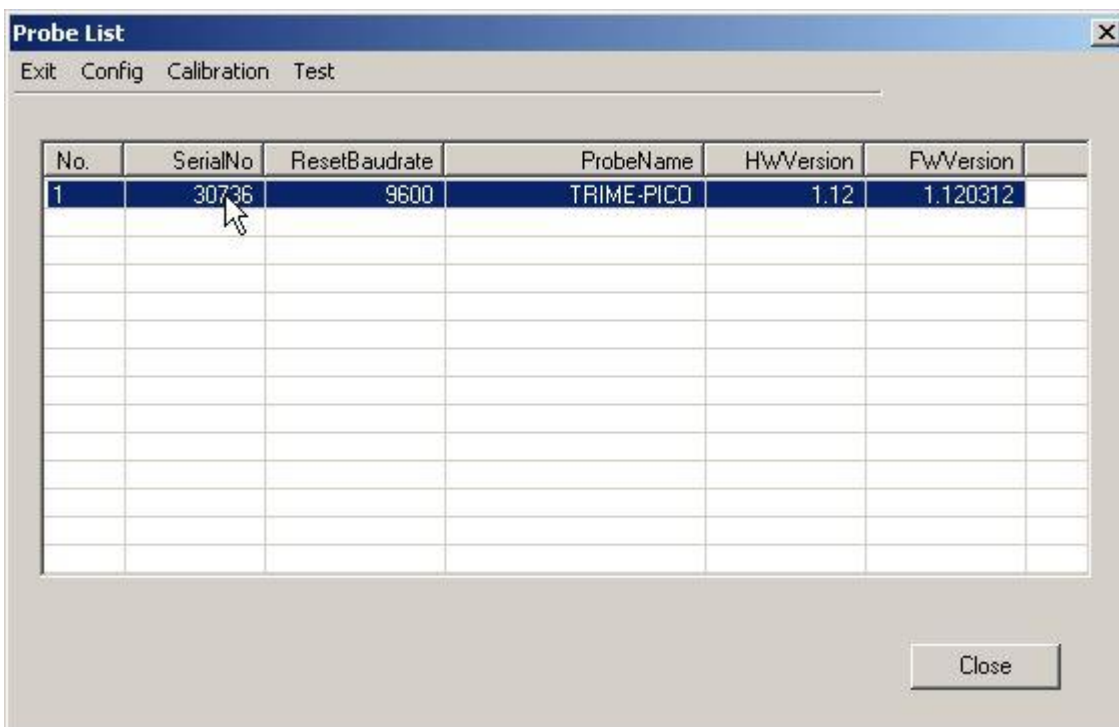


10.4 Configuration of Measure Mode

In "Probe List" with "Config" and "Measure Mode & Parameters" the PICO probe can be adjusted to the desired mode A, B or C (see Chapter "Configuration Measure Mode").

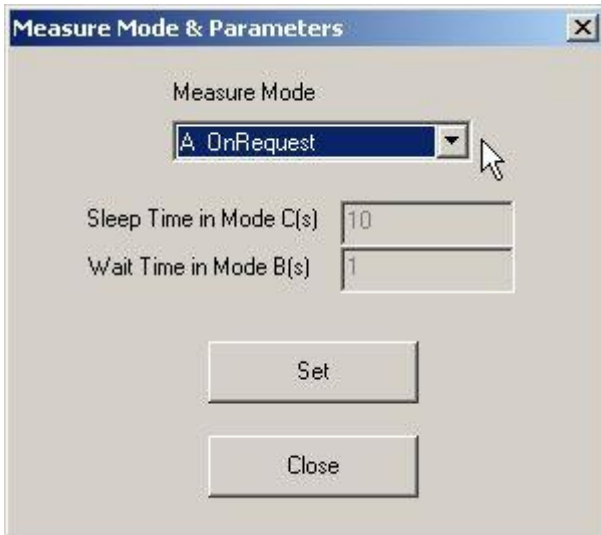

10.5 Analogue outputs of the PICO probe

In the menu "Config" and the window "Analog Output" the analogue outputs of the PICO probe can be configured (see Chapter "Analogue outputs..").

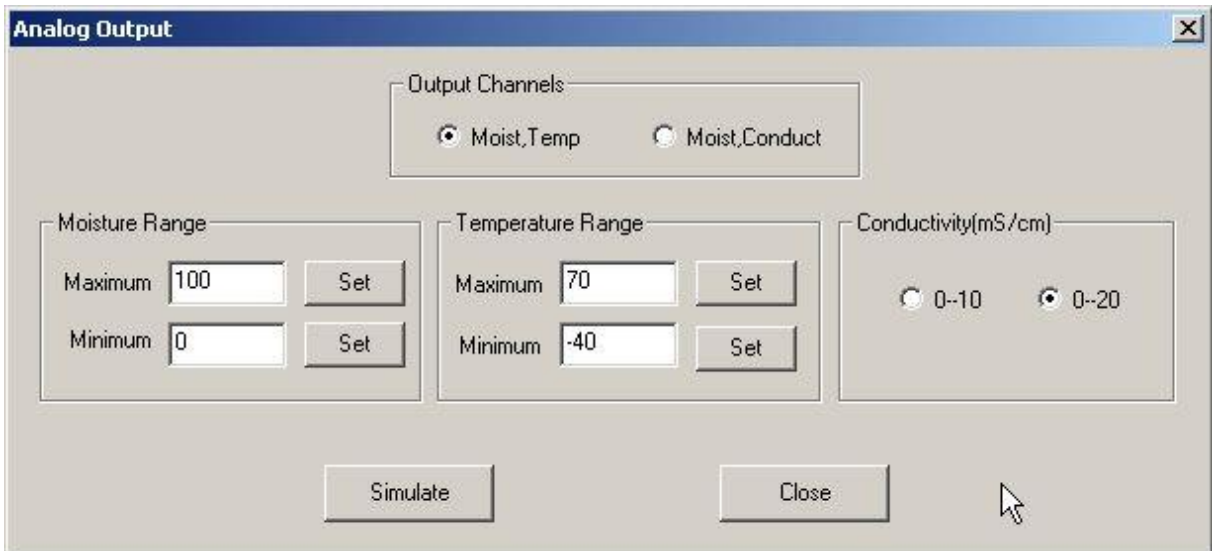


The conductivity range can be selected, depending on the specific soil which is measured. 0..20 dS/m should be selected for soils with a very high salinity content.

10.6 Simulate Analog Output


The PICO PROFILE has no analog outputs! The following text refers to the probes PICO64/32.

By pressing the button **"Simulate"** in the window **"Analog Output"** the analog output 1 and 2 can be simulated in 5 ranges from 0 to 100%. The %-value can be entered directly by hand and the analog output follows by pressing the button **"Set"**.

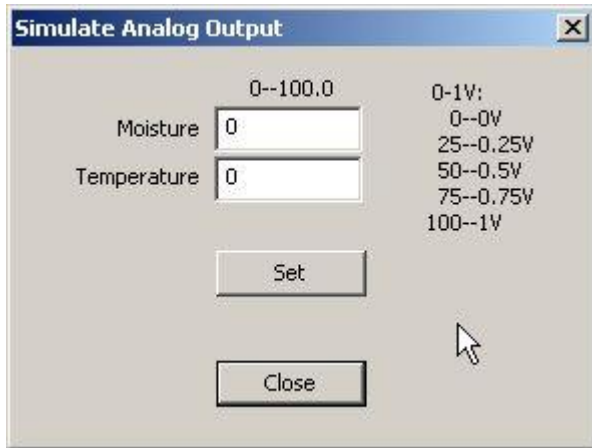

10.7 Selection of the individual Calibration Curves

In the menu **"Calibration"** and the window **"Material Property Calibration"** the calibration curves CAL1 to Cal15 which are stored in the PICO probe are loaded and displayed on the screen (takes max. 1 minute). With the mouse pointer individual calibration curves can be activated and tested with the PICO probe by activating the button **"Set Active Calib"**. Furthermore, the individual calibration curves CAL1 to Cal15 can be adapted or modified with the calibration coefficients (see Chapter **"Creating a linear calibration curve"**).

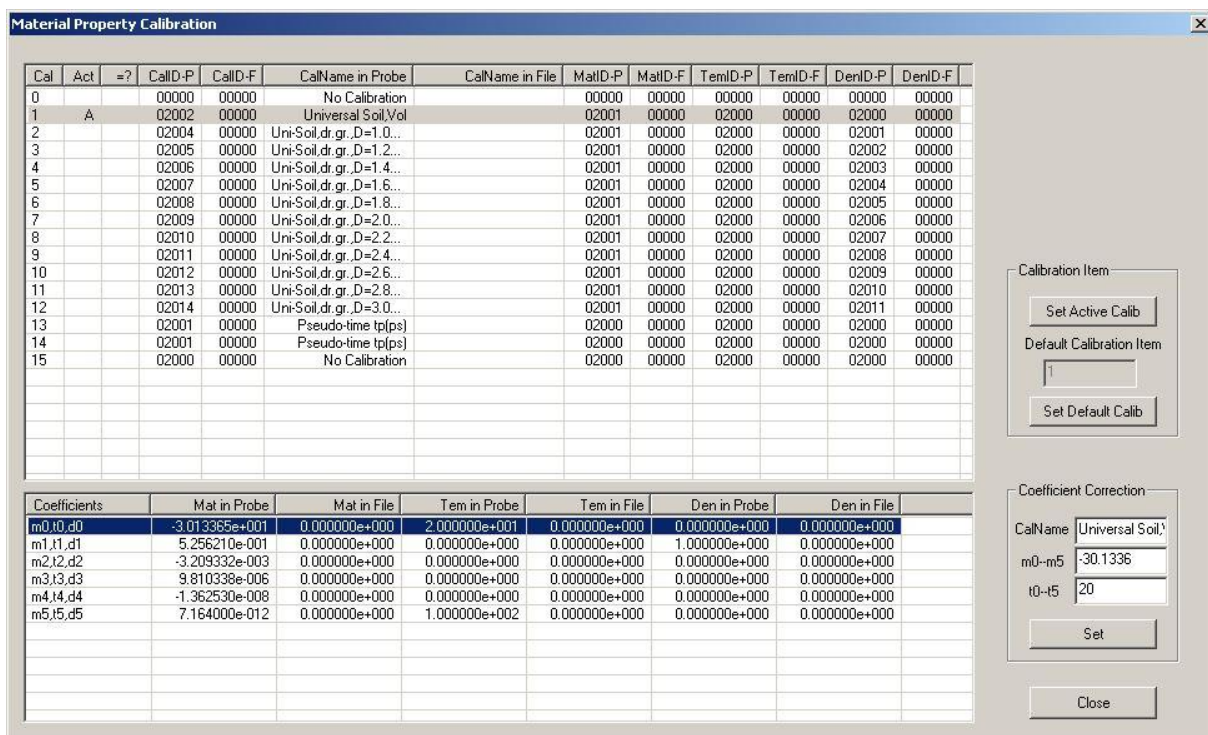

Cal	Act	=?	CallD-P	CallD-F	CalName in Probe	CalName in File	MatD-P	MatD-F	TemD-P	TemD-F	DenD-P	DenD-F
0			00000	00000	No Calibration		00000	00000	00000	00000	00000	00000
1	A		02002	00000	Universal Soil,Vol		02001	00000	02000	00000	02000	00000
2			02004	00000	Uni-Soil,dr.gr.,D=1.0...		02001	00000	02000	00000	02001	00000
3			02005	00000	Uni-Soil,dr.gr.,D=1.2...		02001	00000	02000	00000	02002	00000
4			02006	00000	Uni-Soil,dr.gr.,D=1.4...		02001	00000	02000	00000	02003	00000
5			02007	00000	Uni-Soil,dr.gr.,D=1.6...		02001	00000	02000	00000	02004	00000
6			02008	00000	Uni-Soil,dr.gr.,D=1.8...		02001	00000	02000	00000	02005	00000
7			02009	00000	Uni-Soil,dr.gr.,D=2.0...		02001	00000	02000	00000	02006	00000
8			02010	00000	Uni-Soil,dr.gr.,D=2.2...		02001	00000	02000	00000	02007	00000
9			02011	00000	Uni-Soil,dr.gr.,D=2.4...		02001	00000	02000	00000	02008	00000
10			02012	00000	Uni-Soil,dr.gr.,D=2.6...		02001	00000	02000	00000	02009	00000
11			02013	00000	Uni-Soil,dr.gr.,D=2.8...		02001	00000	02000	00000	02010	00000
12			02014	00000	Uni-Soil,dr.gr.,D=3.0...		02001	00000	02000	00000	02011	00000
13			02001	00000	Pseudo-time tp(ps)		02000	00000	02000	00000	02000	00000
14			02001	00000	Pseudo-time tp(ps)		02000	00000	02000	00000	02000	00000
15			02000	00000	No Calibration		02000	00000	02000	00000	02000	00000

Coefficients	Mat in Probe	Mat in File	Tem in Probe	Tem in File	Den in Probe	Den in File
m0,t0,d0	-3.013365e+001	0.000000e+000	2.000000e+001	0.000000e+000	0.000000e+000	0.000000e+000
m1,t1,d1	5.256210e-001	0.000000e+000	0.000000e+000	0.000000e+000	1.000000e+000	0.000000e+000
m2,t2,d2	-3.209332e-003	0.000000e+000	0.000000e+000	0.000000e+000	0.000000e+000	0.000000e+000
m3,t3,d3	9.810338e-006	0.000000e+000	0.000000e+000	0.000000e+000	0.000000e+000	0.000000e+000
m4,t4,d4	-1.362530e-008	0.000000e+000	0.000000e+000	0.000000e+000	0.000000e+000	0.000000e+000
m5,t5,d5	7.164000e-012	0.000000e+000	1.000000e+002	0.000000e+000	0.000000e+000	0.000000e+000


The desired and possibly altered calibration curve (Cal1. .15) which is activated after switching on the probes power supply can be adjusted with the button "Set Default Calib".

The coefficients $m_1 = 0.0581$ and $m_0 = -4.05$ for individual calibration curves can be entered and adjusted directly by hand and are stored in the probe by pressing the "Set" button.

10.8 Test Run in Measurement Mode A

In the menu "Test" and the window **Test in Mode A**, the measured moisture values "Moist" of the PICO probe are displayed on the screen and can be parallel saved in a file.

Attention: for a test run in mode A it must be ensured that the PICO probe was also set to this mode. If this is not assured, the probe returns zero values.

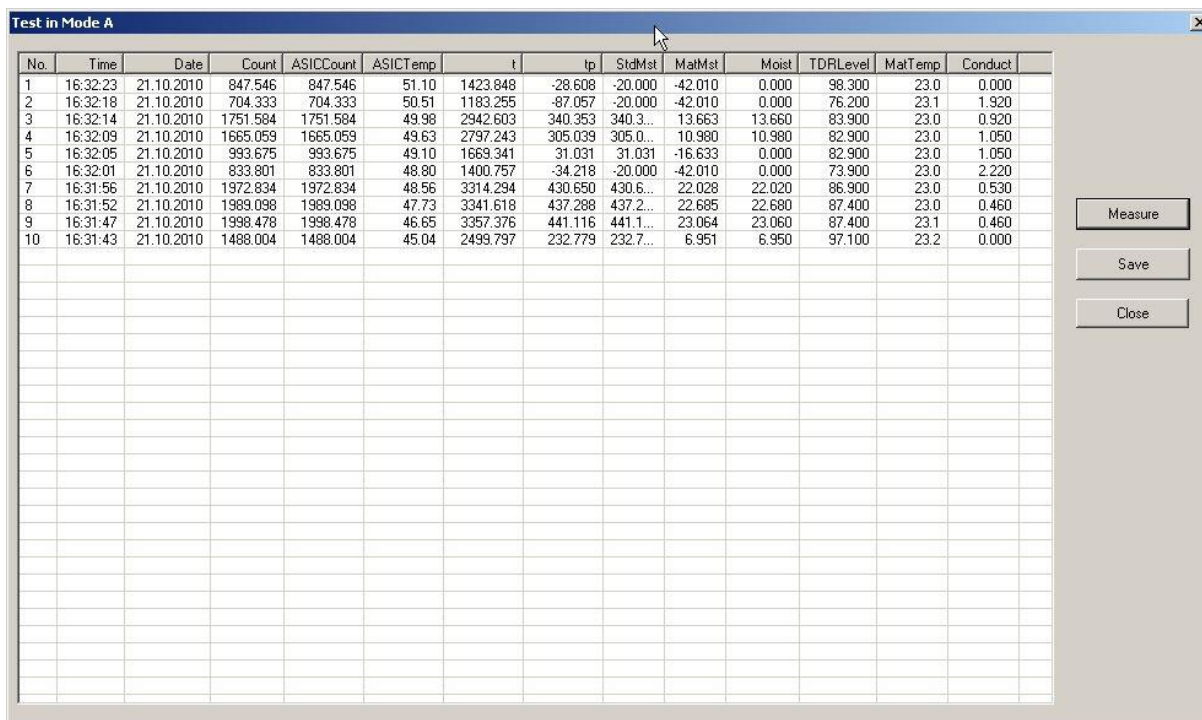

No.	Time	Date	Count	ASICCount	ASICTemp	t	tp	SkdMst	MatMst	Moist	TDRLevel	MatTemp	Conduct
1	16:32:23	21.10.2010	847.546	847.546	51.10	1423.848	-28.608	-20.000	-42.010	0.000	98.300	23.0	0.000
2	16:32:18	21.10.2010	704.333	704.333	50.51	1183.255	-87.057	-20.000	-42.010	0.000	76.200	23.1	1.920
3	16:32:14	21.10.2010	1751.584	1751.584	49.98	2942.603	340.353	340.3...	13.663	13.660	83.900	23.0	0.920
4	16:32:09	21.10.2010	1665.059	1665.059	49.63	2797.243	305.039	305.0...	10.980	10.980	82.900	23.0	1.050
5	16:32:05	21.10.2010	993.675	993.675	49.10	1669.341	31.031	31.031	-16.633	0.000	82.900	23.0	1.050
6	16:32:01	21.10.2010	833.801	833.801	48.80	1400.757	-34.218	-20.000	-42.010	0.000	73.900	23.0	2.220
7	16:31:56	21.10.2010	1972.834	1972.834	48.56	3314.294	430.650	430.6...	22.028	22.020	86.900	23.0	0.530
8	16:31:52	21.10.2010	1989.098	1989.098	47.73	3341.618	437.288	437.2...	22.685	22.680	87.400	23.0	0.460
9	16:31:47	21.10.2010	1998.478	1998.478	46.65	3357.376	441.116	441.1...	23.064	23.060	87.400	23.1	0.460
10	16:31:43	21.10.2010	1488.004	1488.004	45.04	2499.797	232.779	232.7...	6.951	6.950	97.100	23.2	0.000

Following measurement values are displayed on the screen:

- Moist** Moisture Value
- MatTemp** Temperature
- Conduct** Bulk Electrical Conductivity EC_{TRIME}
- TDRLevel** TDR-Level (for special applications)
- tp** Radar time which corresponds to the respective moisture value.

The other values like Count, ASICCount, etc. are for special use.

By clicking „Save“ the recorded data is saved in a text file in the following path:

\PICO-CONFIG.exe-Pfad\MD\Dateiname

The name of the text file **TestMeas+SN+yyyymmddHHMMSS.sts** is assigned automatically with the serial number of the probe (SN) and date and time.

The data in the text file can be evaluated with Windows-EXCEL.

Basic Balancing in Glass Beads

PICO probes are identical and manufactured precisely. After an exchange of a probe rod it is nevertheless advisable to verify the calibration and to check the basic calibration and if necessary to correct it with a “Basic Balancing”.

With a “Basic Balancing” two reference calibration measurements are to be carried out with known set-points (“RefValues”). For the reference media, dry and wet glass beads should be used.

Attention: Before performing a “Basic Balancing” it must be ensured that the PICO probe was set to “Measure Mode” A. If this is not assured, the probe returns zero values. After a “Basic Balancing” the PICO probe has to be set to “Measure Mode” B or C again.


In the menu "**Calibration**" and the window "**Basic Balancing**" the two set-point values of the radar time **tp** are displayed with 145ps and 625ps.

Reference set-point A: **tp**=145ps in dry glass beads.

The first set-point can be activated with the mouse pointer by clicking to No.1. By activating the button "**Do Measurement**" the PICO probe determines the first reference set-point in dry glass beads. In the column „MeasValues“ the measured raw value of the radar time **t** is displayed.

Reference set-point B: **tp**=625ps in wet glass beads. The PICO probe head has to be completely covered with wet glass beads. The second set-point can be activated with the mouse pointer by clicking to No.2. By activating the button "**Do Measurement**" the PICO probe determines the second reference set-point in wet glass beads. In the column „MeasValues“ the measured raw value of the radar time **t** is also displayed.

By activating the button „**Calculate Coeffs**“ and „**Coeffs → Probe**“ the alignment data is calculated automatically and is stored in the PICO probe non-volatile. With a “Test run” (in Mode A) the radar time **tp** of the PICO probe should be now 145ps in dry and 625ps in wet glass beads.

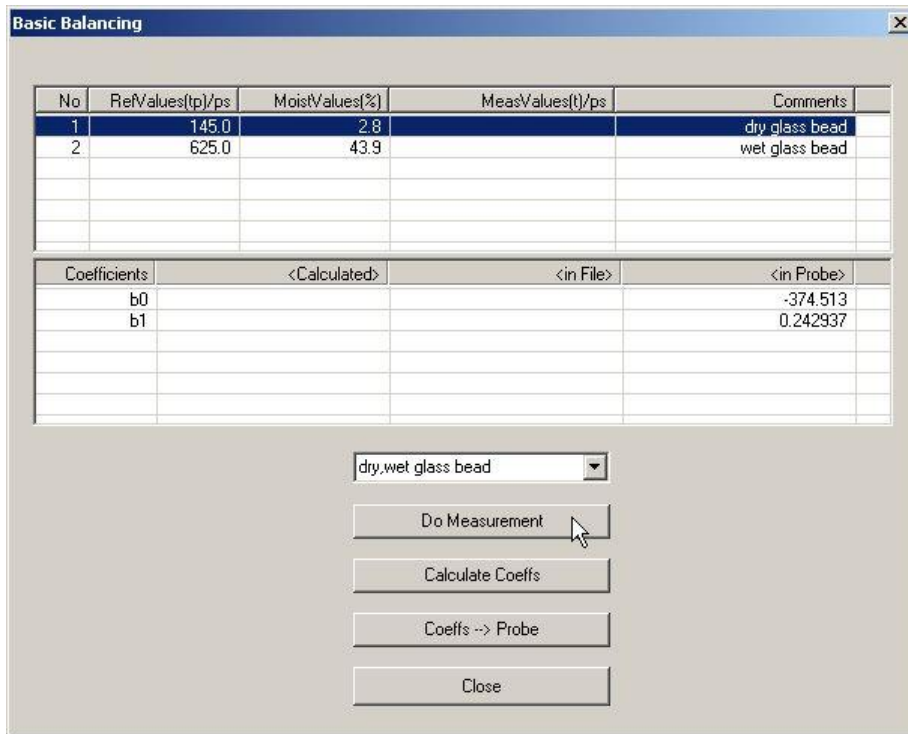

10.9 Calibration Curves

PICO probes are supplied with different calibration curves.

Cal1 Universal Soil Vol. is a nonlinear calibration curve 5th order which is suitable for most soils.

Cal 2 to Cal7 (see next pages) can be selected for special applications. **These are the calibration functions installed to the upgrade version of the TRIME PICO-PROFILE32/64 delivered together with the measurement of the Radar based Conductivity (RbC). If you want to have these Calibration functions for your current TRIME PICO-PROFILE please contact IMKO GmbH (info@imko.de)**

A maximum of 15 different calibration curves (Cal1 ... Cal15) can be stored inside the PICO probe and can optionally be activated via the program **PICO-CONFIG**.

A preliminary test of an appropriate calibration curve (Cal1. .15) can be activated in the menu "**Calibration**" and in the window "**Material Property Calibration**" by selecting the desired calibration curve (Cal1...Cal15) and with using the button "**Set Active Calib**". The finally desired and possibly altered calibration curve (Cal1. .15) which is activated after switching on the probes power supply will be adjusted with the button "**Set Default Calib**".


Nonlinear calibrations are possible with polynomials up to 5th grade (coefficients m0 to m5).

IMKO publish on its website more suitable calibration coefficients for different materials. These calibration coefficients can be entered and stored in the PICO probe by hand (Cal14 and Cal15) with the help of PICO-CONFIG.


Next page:

The following charts (Cal.1 .. 15) show different selectable calibration curves which are stored inside the PICO probe.

On the y-axis the gravimetric moisture **Moist** (or **Dielectric-Constant Epsilon**) is shown. On the x-axis depending on the calibration curve the associated radar time **tp** in picoseconds is shown. With the software **PICO-CONFIG** the radar time **tp** is shown on the screen parallel to the moisture value **Moist**.

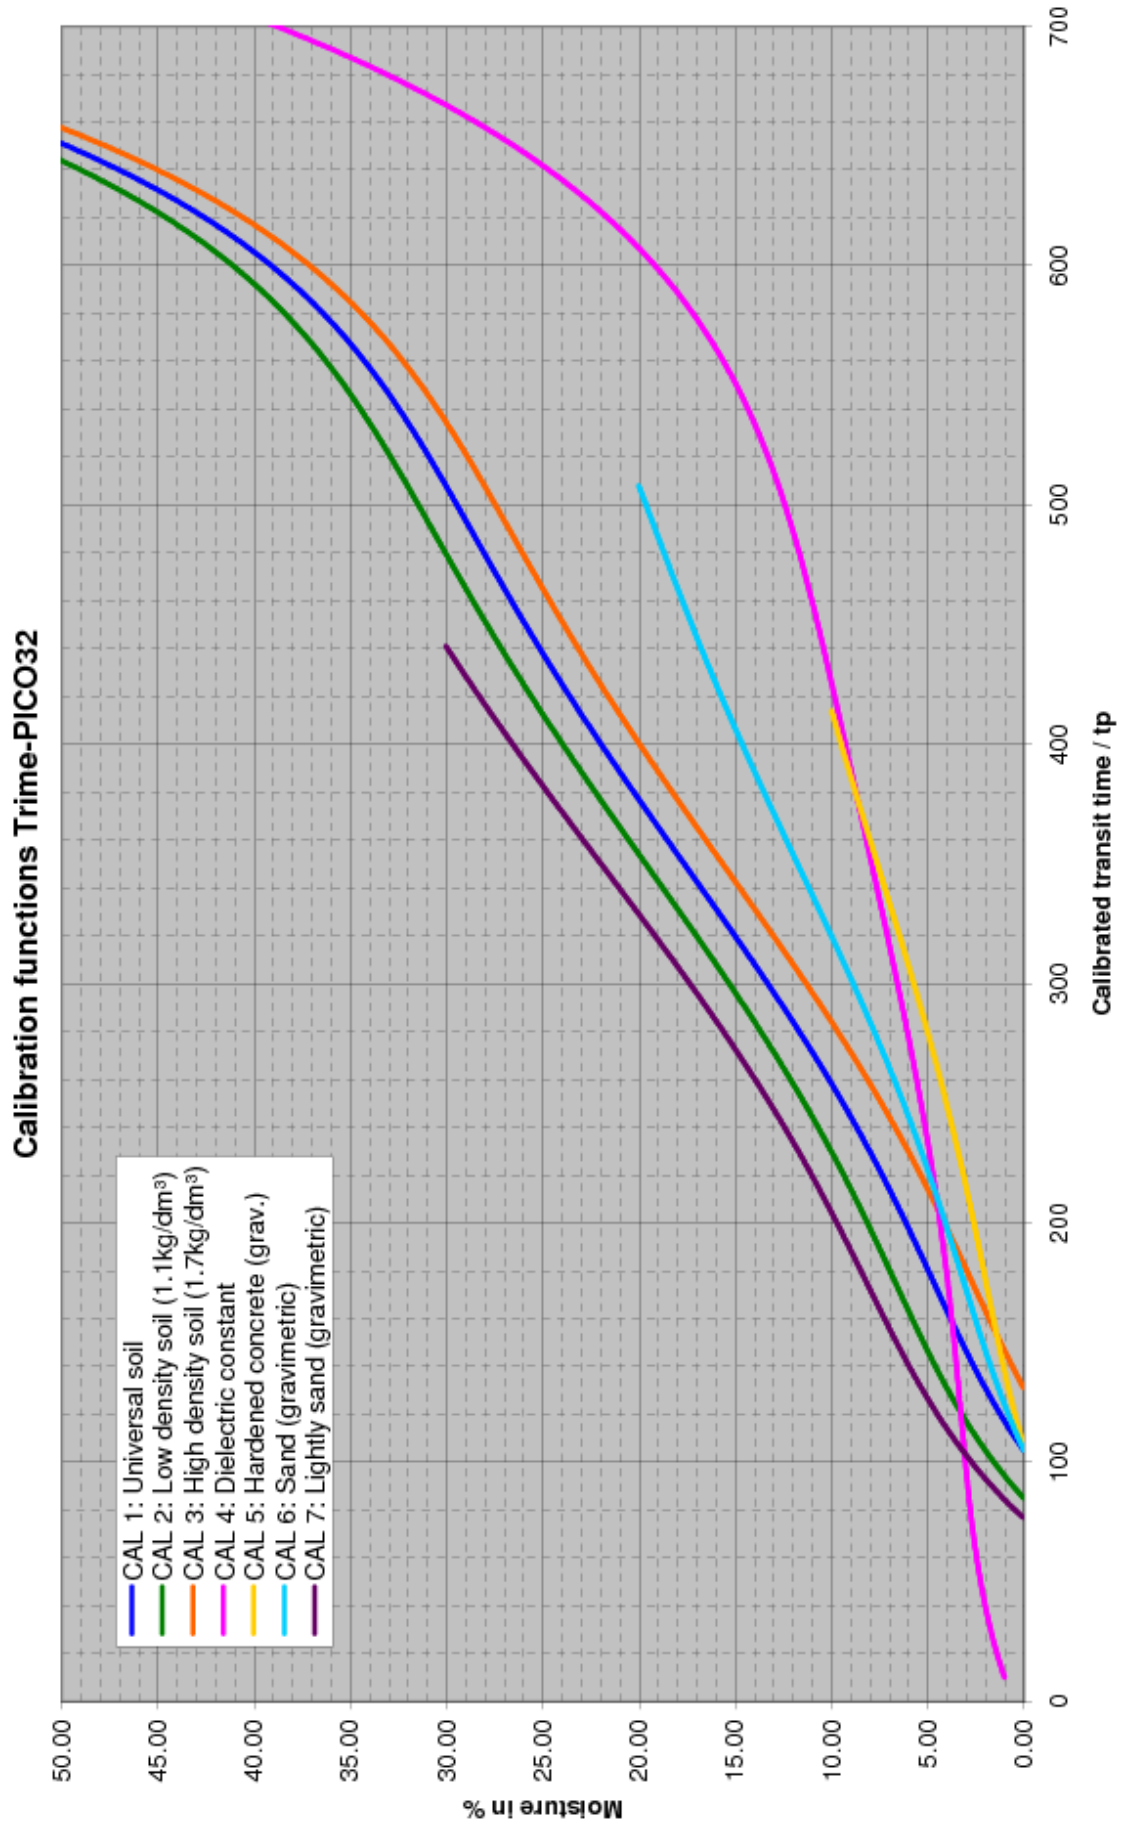

Calibration functions Trime-PICO64

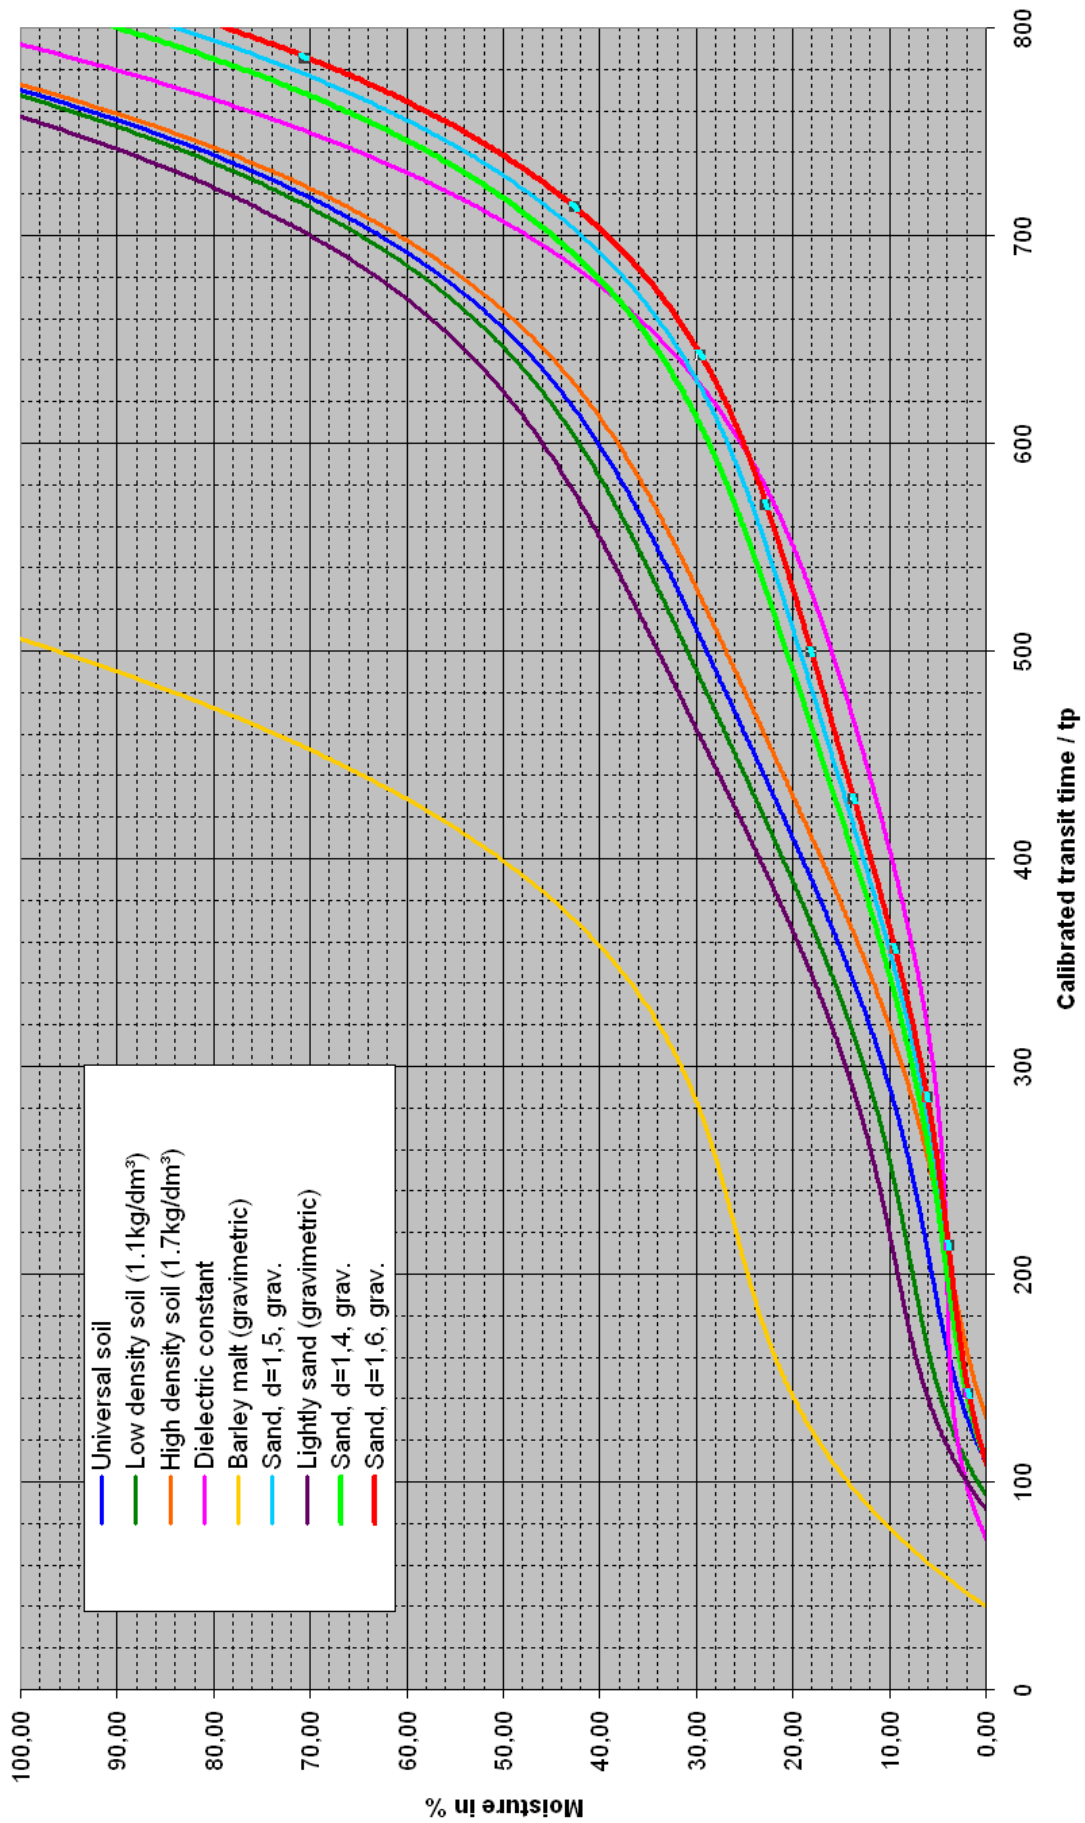

10.10 Creating a linear Calibration Curve for a specific Material

The calibration curves Cal1 to Cal15 can be easily created or adapted for a specific soil with the help of PICO-CONFIG. Therefore, two measurement points need to be identified with the probe. Point P1 at dried soil and point P2 at moist soil where the points P1 and P2 should be far enough apart to get a best possible calibration curve. The moisture content of the soil at point P1 and P2 can be determined with laboratory measurement methods (oven drying). It is to consider that sufficient material is measured to get a representative value.

Under the menu "**Calibration**" and the window "**Material Property Calibration**" the calibration curves CAL1 to Cal15 which are stored in the PICO probe are loaded and displayed on the screen (takes max. 1 minute). With the mouse pointer individual calibration curves can be tested with the PICO-probe by activating the button "**Set Active Calib**". The measurement of the moisture value **Moist** with the associated radar time **tp** at point P1 and P2 is started using the program PICO-CONFIG in the sub menu "**Test**" and "**Test in Mode A**".

Step 1: The radar pulse time **tp** of the probe is measured with dried soil. It is recommended to detect multiple measurement values for finding a best average value for **tp**. The result is the first calibration point P1 (e.g. 70/0). I.e. 70ps (picoseconds) of the radar pulse time **tp** corresponds to 0% moisture content of the material. But it would be also possible to use a higher point P1' (e.g. 190/7) where a **tp** of 190ps corresponds to a moisture content of 7%. The gravimetric or volumetric moisture content of the material, e.g. 7% has to be determined with laboratory measurement methods (oven drying).

Step 2: The radar pulse time **tp** of the probe is measured with moist material. Again, it is recommended to detect multiple measurement values of **tp** for finding a best average value. The result is the second calibration point P2 with X2/Y2 (e.g. 500/25). I.e. **tp** of 500ps corresponds to 25% moisture content. The gravimetric or volumetric moisture content of the material, e.g. 25% has to be determined with laboratory measurement methods (oven drying).

Step 3: With the two calibration points P1 and P2, the calibration coefficients m_0 and m_1 can be determined for the specific soil (see next page).


Step 4: The coefficients $m_1 = 0.0581$ and $m_0 = -4.05$ (see next page) for the calibration curve Cal15 can be entered directly by hand and are stored in the probe by pressing the button "**Set**". The name of the calibration curve can also be entered by hand. The selected calibration curve (e.g. Cal15) which is activated after switching on the probes power supply will be adjusted with the button "**Set Default Calib**".

Attention: Use "dot" as separator (0.0581), not comma !

10.11 Nonlinear calibration curves

PICO probes can also work with non-linear calibration curves with polynomials up to 5th grade. Therefore it is necessary to calibrate with 4...8 different calibration points. To calculate nonlinear coefficients for polynomials up to 5th grade, the software tool TRIME-WinCal from IMKO can be used (on request). It is also possible to use any mathematical program like MATLAB for finding a best possible nonlinear calibration curve with suitable coefficient parameters m_0 to m_5 .

The following diagram shows a sample calculation for a linear calibration curve with the coefficients m_0 and m_1 for a specific soil or material.

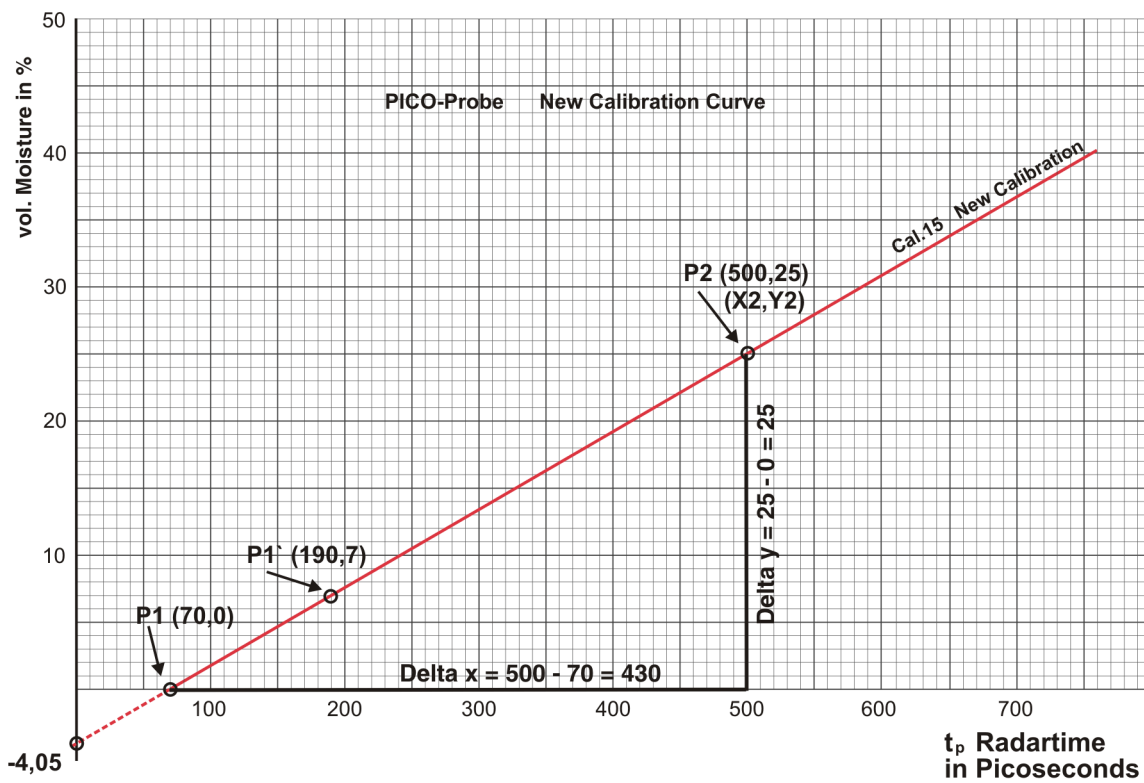

The coefficient m_1 is calculated from the slope of the curve Cal15:

$$\text{Coefficient } m_1 = \frac{\text{Delta } y}{\text{Delta } x} = \frac{25 - 0}{500 - 70} = 0,0581$$

The coefficient m_0 is the offset on the y-axis at $x = 0$:

$$\text{Coefficient } m_0 = Y_2 - (m_1 \cdot X_2) = 25 - (0,0581 \cdot 500) = -4,05$$

11 Electrical Conductivity with TRIME Probes

A reliable, practical and easy-to-use Determination of Soil Conductivity and Salt Content with TRIME Probes

IMKO's TRIME TDR-probes can now report soil EC as standard simultaneously with soil moisture content percentage. A manual conversion based on researched curves for different soil types enables the user to derive a soil EC expressed in mg/l TDS (total dissolved salts).

TRIME TDR probes can do this very accurately because:

TRIME probes measure conductivity with the same large soil volume as it will be used for the TDR moisture measurement. The contact of the probe rods inside the soil is far less critical as with "galvanic" EC probes with a point to point measurement where even small air gaps lead to significant deviations.

TRIME probes use coated and therefore isolated rods which guarantee the non-appearance of galvanic accumulation along the rods allowing for long-run installations over many years. Unisolated rods means there is a risk of galvanic reactions and possible influence on the sensor's reading with serious problems when the probes must be removed from larger depths due to a rod cleaning.

TRIME probes measure moisture and conductivity very precisely at a frequency of 1GHz with a better and more exact separation of moisture and conductivity in comparison to capacitive probes with lower frequencies. This means that in practice, a reliable determination of the pore water conductivity EC_w and respectively TDS (mg of salt per liter water) is possible at different moisture levels.

All TRIME probes work with a concurrently basic calibration for moisture and conductivity. This allows a check of the limits of saline stress in soils according to standards of FAO2006 for specific soils.



11.1 The analysis of Soils for Electrical Conductivity EC_{TRIME}

Notes and Disclaimer: The analysis of electrical conductivity is an immensely complex subject. This resume is not intended as a study document in soil science nor does it discuss the technical complexities of the devices used.

For agricultural and horticultural soils, the measurement of Electrical Conductivity is an immensely important measurement. Electrical Conductivity measures the amount of total dissolved salts (TDS) or total dissolved ions in water. To complicate matters, some ions such as Sodium and Chloride will contribute more to EC than others such as Phosphorus and Potassium.

Plants require nutrients such as Nitrogen, Phosphorus, Potassium, Magnesium in large quantities hence they are called major nutrients and also smaller amounts of elements such as Iron, Manganese, Molybdenum and these are called micro nutrients or sometimes referred to as trace metals. Fertilisers are supplied to plants as compounds for example Ammonium Nitrate which supplies Nitrogen in the form of Nitrate or Ammonium. Micro-organisms will break down these compounds so they are more readily available for uptake by the plants. Levels of some ions such as Chlorides are less desirable and in great quantities can be harmful to plant growth. The quantity of ions or salts in a soil is of huge importance. Too much or too few nutrients will create a restriction in plant growth.

Measurement of EC in water is relatively straightforward. An EC probe (usually platinum) is inserted in the water and a reading in mS/cm is reported on the meter's display. This is relatively easy because water is a homogeneous medium. Soil on the other hand is not and this has caused great difficulties when trying to measure its conductivity. To work around this, the analysis on agricultural and horticultural soils has been carried out by mixing a volume of soil and a volume of water and measuring the EC on the suspension or filtered extract. Different countries and different regulatory bodies have specified methodologies and in general results have been good enough to use for fertilisation recommendations and programmes. This analysis was generally carried out by a laboratory and whereas results were and are reliable the method is slow, time consuming and expensive.

Over the years manufacturers have tried to come up with solutions whereby an instrument could be used directly in soils without having to resort to laboratories. The EC reported by these instruments is referred to soil bulk electrical conductivity. Whereas there has been some success, there are so many influential variables such as temperature, soil moisture and granular composition that results have not been adequate for reliable fertilisation studies. Mostly soil bulk conductivity was of academic rather than practical interest.

IMKO has studied the subject in detail and has come up with a breakthrough. By using coated rods and measuring over the length of the probes, all TRIME probes can now accurately report what IMKO calls EC_{TRIME}. This measurement takes account of soil moisture and conductivity by volume. Because soil moisture is so important in the calculation of EC, all different TRIME probes now incorporate TDR calibration curves for a selection of soils. Special graphs have been constructed so that the user can convert the EC_{TRIME} reading to grams/litre of dissolved salt. So far curves are available for sandy and loam soils and it is intended to produce a handful of curves to cover most situations. At this moment in time, conversion of EC_{TRIME} to mg/l TDS is done manually.

IMKO hopes that this breakthrough whereby a TDR instrument can be used to derive a true soil EC measurement will become the new standard for soil fertilisation analyses.

11.2 EC_{TRIME} Measurement Range for TRIME Probes

All PICO probes work with a concurrently basic calibration for moisture and conductivity. This allows a check of the limits of saline soils according to standards of FAO2006 for specific soils.

Measurement Range Conductivity for PICO64, PICO32, T3-IPH, PICO-PROFILE

0...10dS/m EC_{TRIME} (here is, depending on moisture content EC_w >20dS/m)

All TRIME probes have a linear EC_{TRIME} calibration curve with two calibration points. This ensures an equal behaviour of a TRIME probe type (e.g. PICO32).

Calibration Point1: Dry glass beads = 0dS/m EC_{TRIME}

Calibration Point2: Saturated glass beads with water EC_w 5dS/m = 5dS/m EC_{TRIME}

With dry glass beads (not air!) it is ensured that the conductivity range of dry soils starts with nearly 0dS/m. The calibration at point2 was performed with glass beads and water which was adjusted with salt to a pore water conductivity of $EC_w = 5dS/m$ at a temperature of 23°C.

11.3 Measurement of Pore-Water-Conductivity or Salt-Content of Soils

The possible salt stress depends on soil type and plant species and can be roughly classified:

Slight salinization:	1-3g of salt per liter
Average salinity:	3-5g salt / liter
Strong salinity:	5-10g salt / liter
Very high salinity:	> 10 g salt / liter

The conversion of the salt content in grams of salt per liter water (TDS Total-Dissolved-Salts) into the pore water conductivity of EC_w happens with:

Salt content in grams of salt per liter of water $TDS = 0.64 * EC_w$

An $EC_w = 5mS/cm$ result thus with 3.2 grams of salt per liter (pore) water


EC_w can be determined with a laboratory conductivity meter. 1dS/m = 1mS/cm

A determination of the pore water conductivity or salinity of soils and sand at different moisture values is possible by using a Moisture/ EC_{TRIME} diagram for the PICO32 or PICO64. With measuring moisture and EC_{TRIME} , the pore water conductivity (or TDS salt content in grams salt per liter) of the soil can be determined by using the individual pore water curves.

The below displayed Moisture/ EC_{TRIME} charts were created for sand and a loamy soil.

We recommend the creation of a separate Moisture/ EC_{TRIME} diagram for the intended soil in the designated ranges of salinity.

The following diagram illustrates curve progressions of pore-water with four different salinity contents at different moisture contents for the PICO32. Sand1 was mixed with 0,5dS/m pore water, sand2 mixed with water which had a conductivity of 5dS/m, sand3 with 10dS/m and sand4 with 20dS/m water. The PICO32 determines different EC_{TRIME} conductivities in the different sands at one moisture level. The moisture range with the best resolution for the EC_{TRIME} measurement lies between 10% and 30%, depending on the salt content.

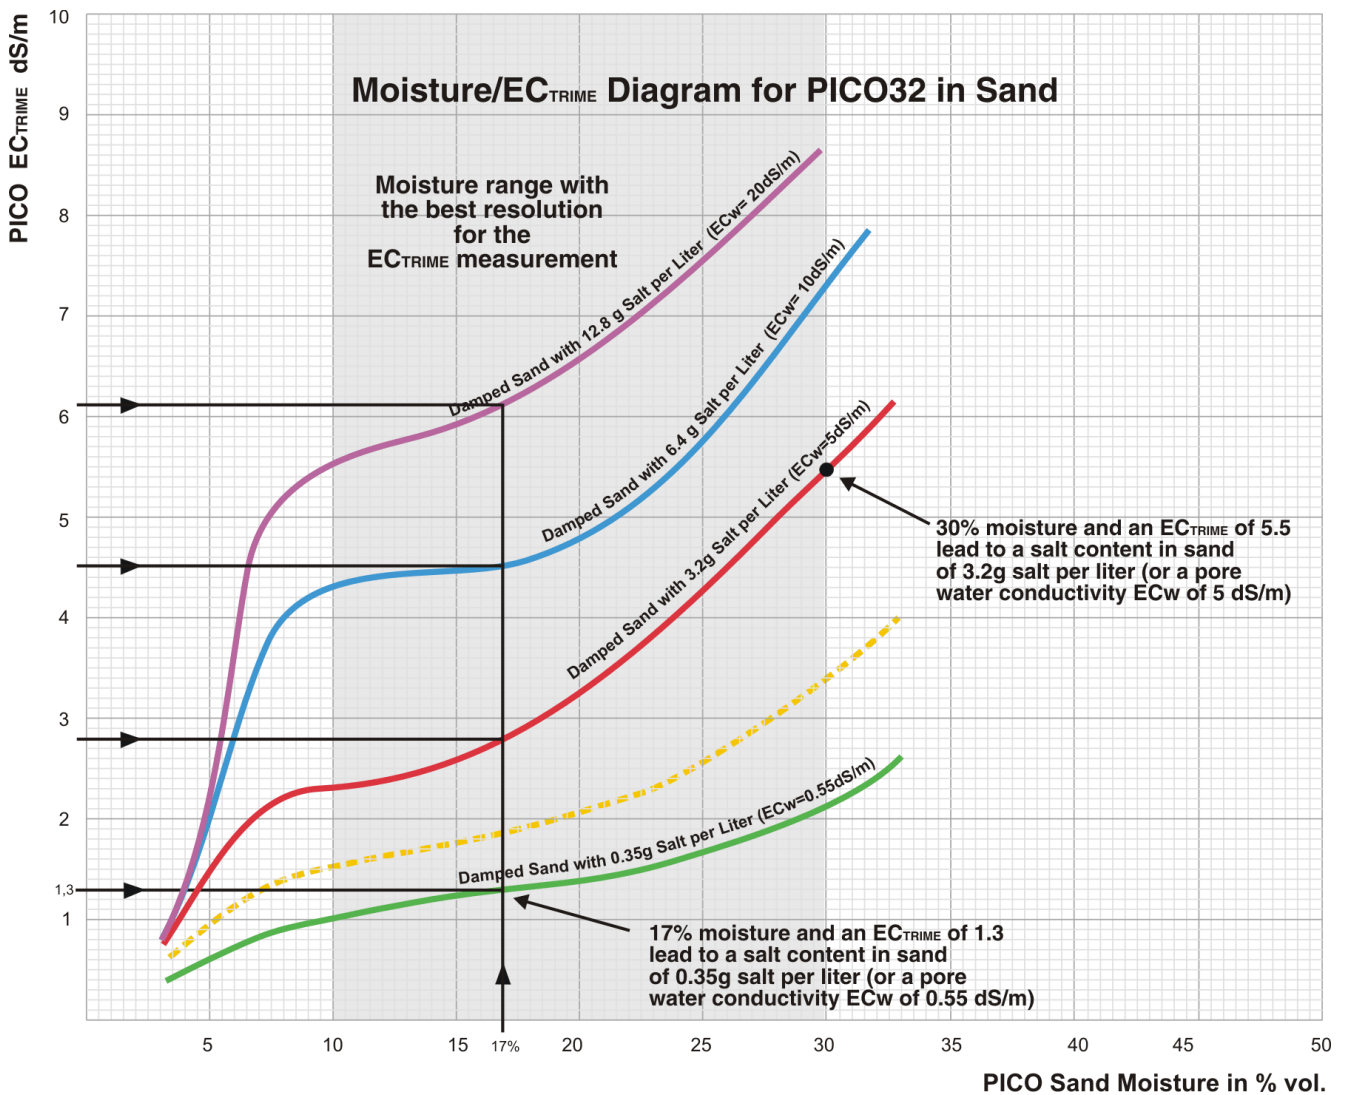


How to determine the salt content

With both parameters, the moisture value and EC_{TRIME} it is possible to determine the salt content in sand. With a moisture content of e.g. 17% and an EC_{TRIME} of 4,6dS/m, the intersection point lies on the blue curve which represents a salt content of 6,4g salt per liter water in the sand. With 30% moisture content and an EC_{TRIME} of 5,5dS/m the salt content would be 3,2g salt per liter water in the sand.

This sand diagram shows four pore water curves. If intersection points lies between this four curves (e.g. the yellow curve), the result of the salt content has to be interpolated.

The following diagram illustrates curve progressions of EC_{TRIME} for PICO32 for a loamy soil at different salt contents. The PICO32 determines different EC_{TRIME} conductivities in different soils at one moisture level. The moisture range with the best resolution for the EC_{TRIME} measurement for a loamy soil is between 25% and 35%.

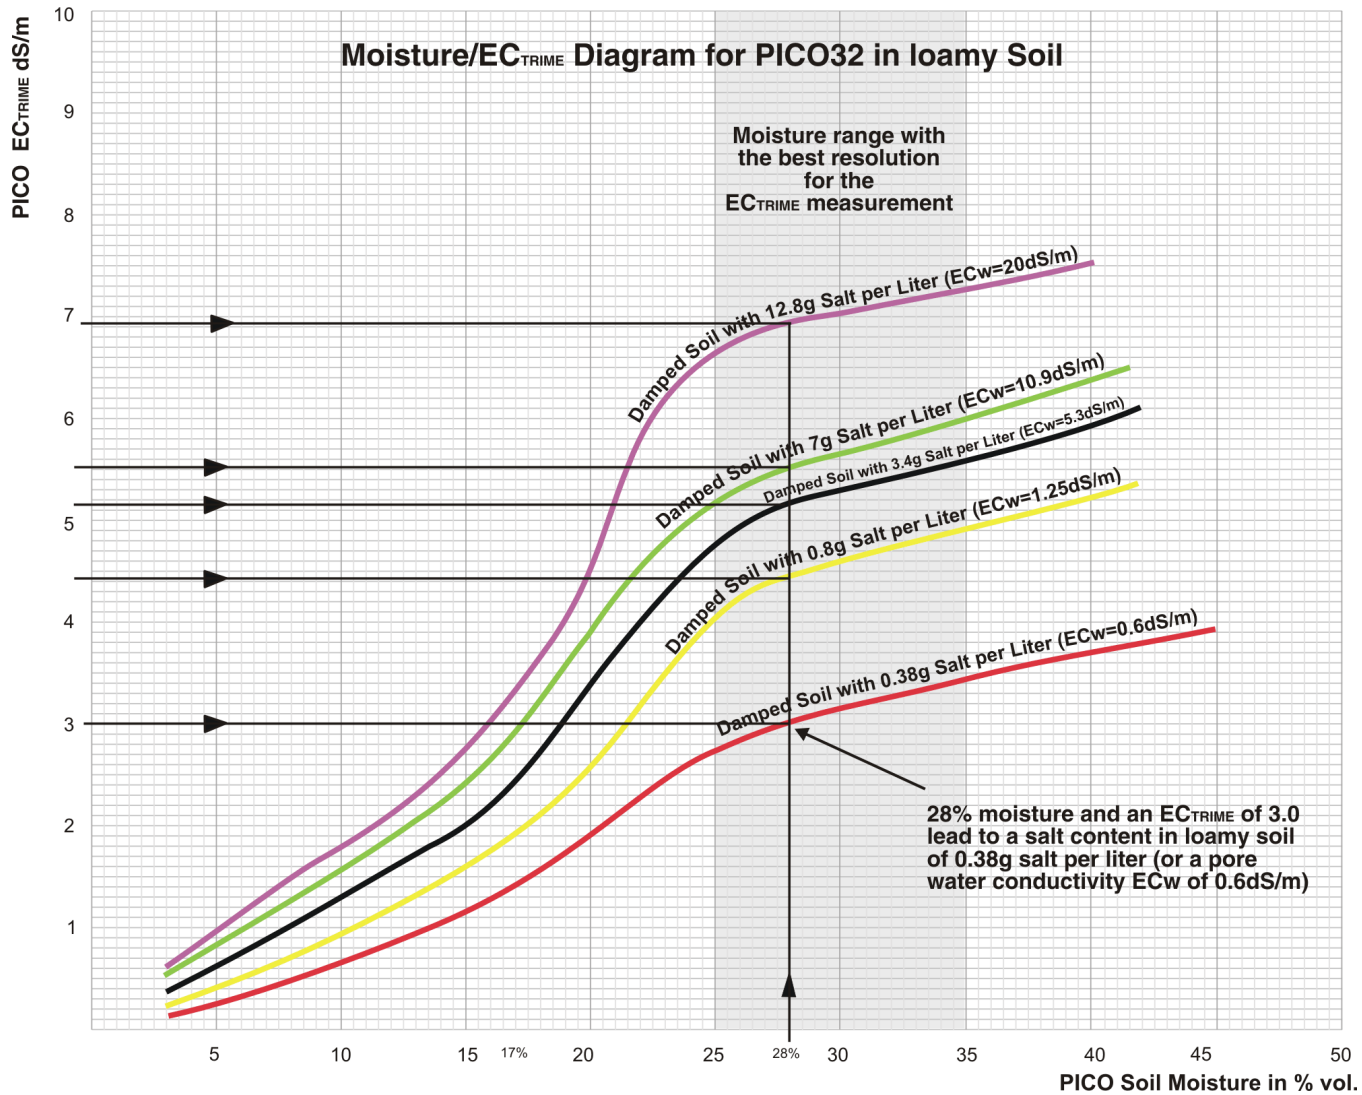

11.4 Creation of a Moisture/ EC_{TRIME} Diagram for a particular Soil

The following description shows a possible way to create a Moisture/ EC_{TRIME} diagram for a particular soil:

Take a soil sample and determine the salt content with a laboratory method. (e.g. determine EC_w of the soil/water saturation extract).

Dry the soil sample to 0% moisture. Cut it into small pieces and grind the soil so that it can be moistened by hand as evenly as possible (eg with a water spray pump).

Moisten the soil evenly with a pore water solution for example 2.56g of salt per liter (equivalent to $EC_w = 4\text{dS/m}$) to the first measurement point (e.g 2.5% moisture). Take into account, that the soil already contains salt. I.e. were already 1g of salt per liter in the soil, you put a curve for a pore water conductivity record of 2.56 g + 1g salt = 3.56g per liter ($EC_w = 5.5\text{ dS/m}$).

Compact the soil in a plastic bowl (no metal and not too small!) so that it largely corresponds to the natural density. Concerning the insertion of the PICO-probe rods for measurement, it is recommended to perform several measurements per point in order to form an average value for each moisture and EC_{TRIME} value. It is important to ensure that the measuring field is not disturbed around the rods, eg by previous punctures.

Moisten the soil more, as homogeneous as possible with the pore water solution $EC_w = 4\text{dS/m}$ to eg 5% moisture. Again compact the soil in a plastic bowl so that it largely corresponds to the natural density. Concerning the insertion of the PICO-probe rods for measurement, it is recommended to perform several measurements per point in order to form an average value for each moisture and EC_{TRIME} value. It is important to ensure that the measuring field is not disturbed around the rods, eg by previous punctures.

Take more moisture and EC_{TRIME} values, up to soil saturation.

Create the pore-water curve for example for 3.56g salt/liter ($EC_w = 5.5\text{dS/m}$) with the added moisture and EC_{TRIME} values.

Take up several curves for different pore water contents.

If the soil sample is already too heavily loaded with salt, a washing out of the ions would be possible, but without the loss of the fine fraction. After a subsequent drying and crushing of the soil, the Moisture/ EC_{TRIME} diagram can be established with a lower salt content. It is also possible to use distilled water for obtaining the lowest curve.

Note: The effort for a Moisture/ EC_{TRIME} diagram is not negligible. IMKO has the hope to establish with the EC_{TRIME} process an easier, faster, better and generally accepted determination of the salt contamination of soils. In future IMKO plans to provide or publish different Moisture/ EC_{TRIME} curves for standard soils. We expect to cover nearly most soils with about 4-5 diagrams.

12 Software Error codes

12.1 Software Errors which will be coded with 4 digits.

Code	Explanation	Measurement
0101-0108, 0301	Serial Port errors	Check port's setting or if the port has been opened. Then close and restart the program.
0201	No answer	Check the power of PICO, the serial port of PC and the connection between PC and PICO.
0202-0212	Protocol errors	Check if PICO-CONFIG's version passes PICO's version.
0302-0307	Protocol error, Parameter setting false	Check if parameters are correct and if PICO-CONFIG's version passes PICO's version.
0401	Can not find config file PICO-CONFIG.con	Look for the file in the exe path. If not found, copy the file to the path.
0501-0508	Errors in Event & MeasureMode	Restart PICO and PICO-CONFIG
0601,0602,0604, 0605,0606,0607, 0609	Operation errors in Basic Balancing	Operate correctly and try it again.
0603,0608,0610, 0611	Communication or protocol errors in Basic Balancing	Restart PICO and PICO-CONFIG.
0701,0702	Read file errors in Material Property Calibration	Check if the files are in the required path. If not, copy the files to the path or redefine the path under the menu Bus/Configuration/Material Property Calibration.
0703	Operation errors in Material Property Calibration	Operate correctly and try it again.
0704, 0705,0706	Communication or protocol errors in Material Property Calibration	Restart PICO and PICO-CONFIG.
0801-0805,0901	Operation errors in Calibration IDs and Names	Operate correctly and try it again.
1001,1101,1102	Read file errors in Calibration IDs and Names	Check if the files are in the required path. If not, copy the files to the path or redefine the path under the menu Bus/Configuration/Material Property Calibration.

1201, 1203	Operation errors in Test	Operate correctly and try it again.
1202	Communication or protocol errors in Test	Restart PICO and PICO-CONFIG.
1301	Write file error in Test	Check file path and try it again. If failed, restart PICO-CONFIG.
4001-4002, 4101-4106,4201	Read file or write file errors	Check the files and try again.
4301-4303	Intenal calculating errors	Restart PICO-CONFIG and try again. Otherwise contact IMKO.

12.2 PICO Errors (Firmware errors)

The errors come from the firmware, from 1 to 255.

Code	Explanation	Measurement
1-19	The serial communication errors due to incorrect telegram, baud rate, timing etc.	Power off, power on PICO and try it again. Otherwise contact IMKO.
20-39	incorrect command number, command right or command parameters.	Power off, power on PICO and try it again. Otherwise contact IMKO.
40-49	EEPROM is defect	Power off, power on PICO and try it again. Otherwise contact IMKO.
50-59	ASIC is defect	Power off, power on PICO and try it again. Otherwise contact IMKO.
60	Power voltage is too low	Check power voltage of PICO, it is minimal 6V.
100	TDR measurement parameter is incorrectly set or the material conductivity is too high.	Adjust the TDR measurement parameters or contact IMKO
101	TDR measurement parameter is incorrectly set	Adjust the TDR measurement parameters or contact IMKO
102	ASIC is defect	Power off, power on PICO and try it again. Otherwise contact IMKO.
103	EC parameter is incorrectly set.	Power off, power on PICO and try it again. Otherwise contact IMKO.
105	TP is out of range for the standard calibration polynomial.	Check if PICO is inserted in the measured material correctly.
108	TDR measurement parameter is incorrectly set or the material conductivity is too high.	Adjust the TDR measurement parameters or contact IMKO
120-129	Internal chip problem	Power off, power on PICO and try it again. Otherwise contact IMKO.
130-199	Internal errors	Contact IMKO
200-254	Reserved	
255	The data transmission is not finished.	

Precise Moisture Measurement

**in hydrology, forestry, agriculture, environmental and earth science,
civil engineering, as well as individual applications!**